SCOTTSDALE POLICE DEPARTMENT CRIME LABORATORY BLOOD ALCOHOL FACE SHEET

ANALYSIS DATE	7/10/18	SEQUENCE NA	ME 10JUL18	
EQUIPMENT		Weylin:	·C·7.	
Pipettor Gas Chromatograph	Hamilton ML600EH Agilent US1417302	H7497 A Hamilton Hamilton A Hamil	ML600GJ10749	
INSTRUMENT CALIBI	Agilent US1417302 RATION	ieuthonic disservi	BILL	
Vial 1 0.02 calibrator Lot	FN03247604	author dispersion of author di	fficient of determination (r²)	
Vial 2 0.10 calibrator Lot	FN06181501 CO	50/19 19	0.99995	
Vial 3 0.20 calibrator	FN07201502	eno cutor		
Vial 4 0.40 calibrator Lot	FN11191402	rosecutor		
Just	cle "tho" City			
CALIBRATION VERIF	CATION AND R	ESOLUTION TES	<u>T</u>	
Vial Sample	Expected result	Measured result	Manufacturer/lot	
5 Blank	Not detected	Not detected	SPD lab 042518	
6 Volatiles mixture	6 compounds	6 compounds	SPD lab 020917WLA	
7 Aqueous control	0.400 g/dL	0.399 g/dL	Lipomed 08012015-C	
8 Aqueous control	0.040 g/dL	0.040 g/dL	Lipomed 09022015-A	
9 Blood control	0.198 g/dL	0.198 g/dL	ACQ 407041529/3	
20 Aqueous control	0.080 g/dL	0.080 g/dL	Lipomed 28082014-B	
31 Aqueous control	0.150 g/dL	0.152 g/dL	Lipomed 09022015-D	
42 Blood control	0.198 g/dL	0.198 g/dL	ACQ 407041529/3	
53 Aqueous control	0.080 g/dL	0.081 g/dL	Lipomed 28082014-B	
58 Aqueous control	0.400 g/dL	0.407 g/dL	Lipomed 08012015-C	
59 Aqueous control	0.040 g/dL	0.041 g/dL	Lipomed 09022015-A	
60 Blood control	0.198 g/dL	0.200 g/dL	ACQ 407041529/3	
61 Blank	Not detected	Not detected	SPD lab 042518	
SUBJECT SAMPLES				
Subjects in the sequence _	22 Su	ıbjects requiring reana	lysis0	
ADDITIONAL NOTES: All	testing proceeded as	s expected.		
Run valid ⊠ Run invalid □		Run valid 🗹 🙏	B1570 7/12/18	
/ Áń:	alyst		Technical Reviewer	

Scottsdale Police Department Crime Laboratory Sequence Quality Assurance Summary

SEQUENCE NAME: 10JUL18


AN	ΑL	YS	T:	Ra	ines
----	----	----	----	----	------

W

Sample Name	Vial	Measured Value (g/dL)	Expected Value (g/dL)	Percent Difference	Absolute Difference (g/dL)
blank 042518	5	negative	negative	Mois P	-
0.400 Lipomed 08012015-C	7	0.399	0.400	0.25	-0.001
0.040 Lipomed 09022015-A	8	0.040	00040	0.00	0.000
0.198 ACQ 407041529/3	9	0,198	0,1985	0.00	0.000
0.080 Lipomed 28082014-B	20	60.080	0.080	0.00	0.000
0.150 Lipomed 09022015-C	31,	0.182	0.150	1.33	0.002
0.198 ACQ 407041529/3	42	20 .198	6 198	0.00	0.000
0.080 Lipomed 28082014-B	53	S 0:080	0.080	1.25	0.001
0.40 Lipomed 08012015-C	58	0.407	0 400	1.75	0.007
0.04 Lipomed 09022015-A	59	0.041	0.040	2.50	0.001
0.198 ACQ 407041529/3	60	0.200	0.198	1.01	0.002
blank 042518	61	negative	negative	<u>-</u>	-

Calibrator	Ethanol Area	N-propanol Area	Ratio
5 0.020	12.118	164.633	0.074
0.100	63.664	170.304	0.374
0.200	123.448	163.544	0.755
0.400	245.829	160.684	1.530

Calibration Line

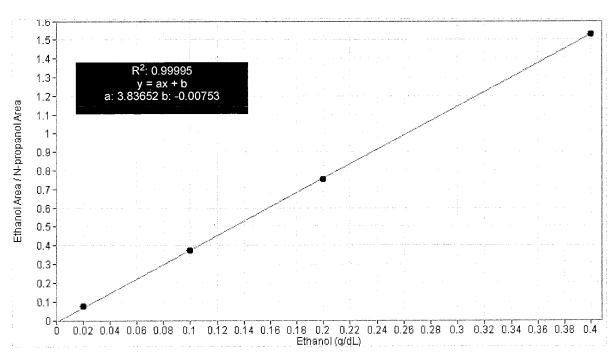

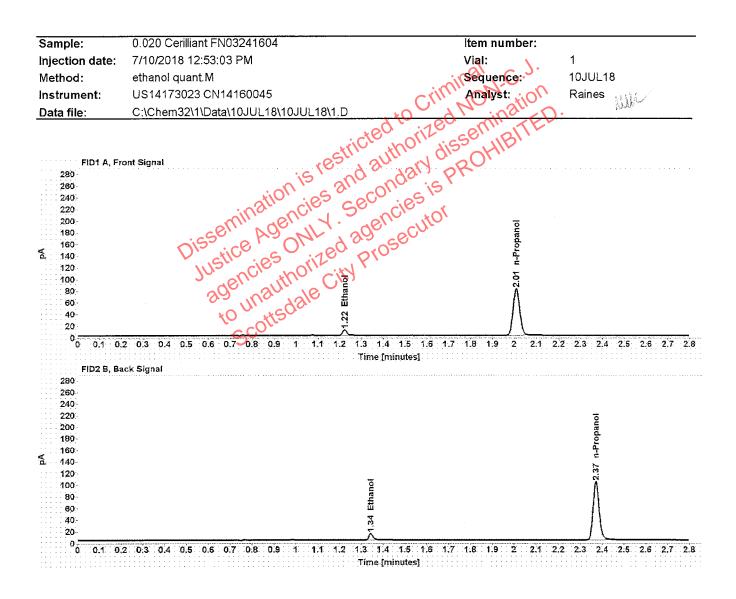


Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.223	12.118
n-Propanol	2.010	164.633

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.344	14.006
n-Propanol	2.371	192.317

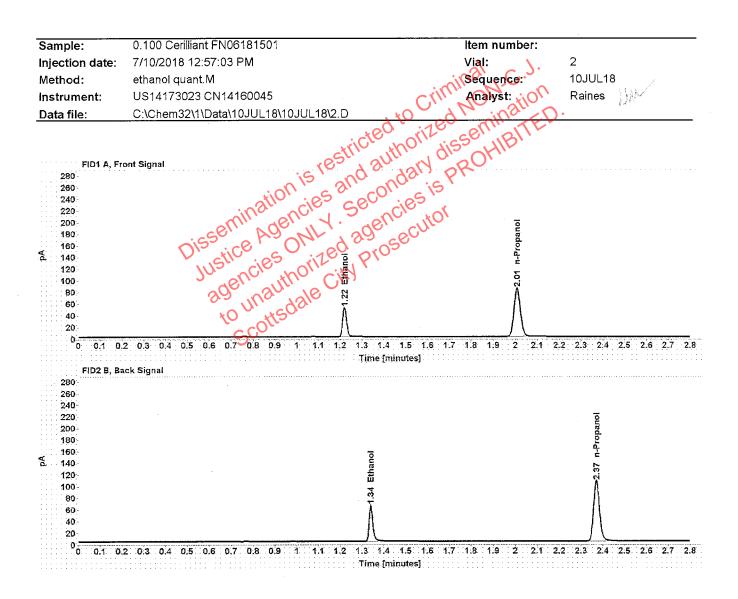


Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.220	63.664
n-Propanol	2.009	170.304

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.340	75.095
n-Propanol	2.370	199.391

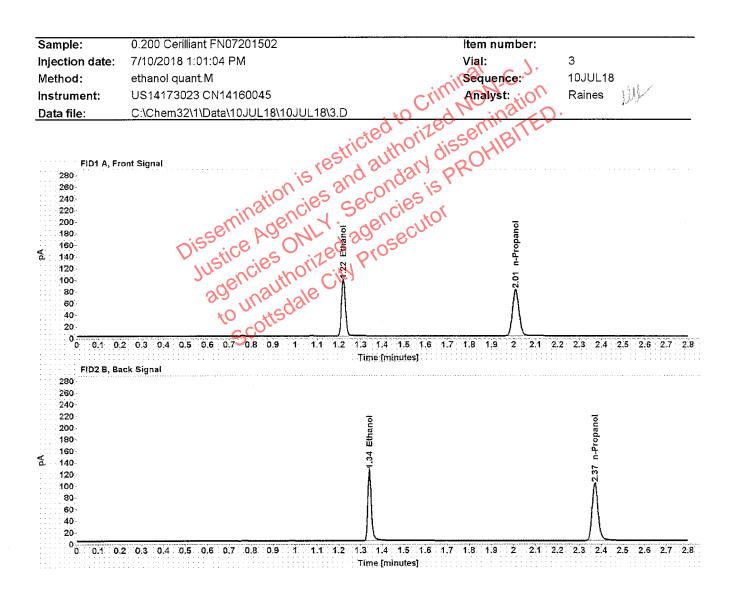


Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.220	123.448
n-Propanol	2.009	163.544

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.340	147.446
n-Propanol	2.371	191.231

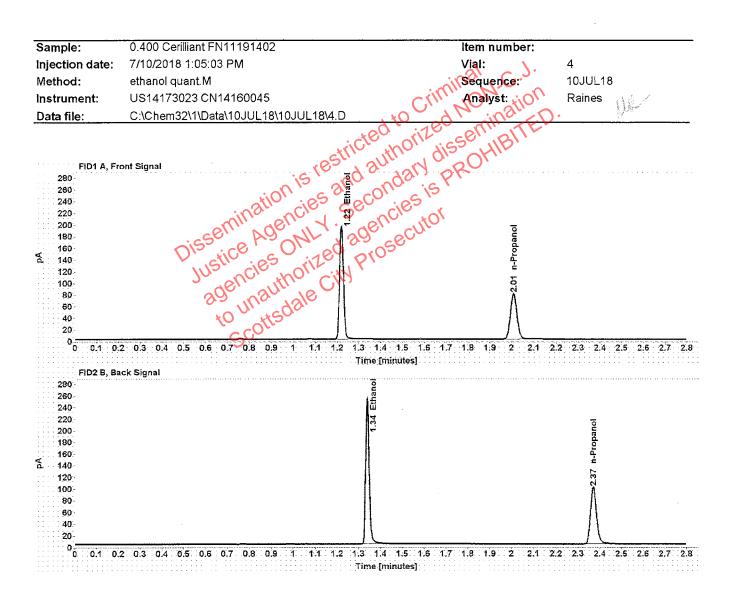


Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.219	245.829
n-Propanol	2.009	160.684

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.339	295.521
n-Propanol	2.371	187.789

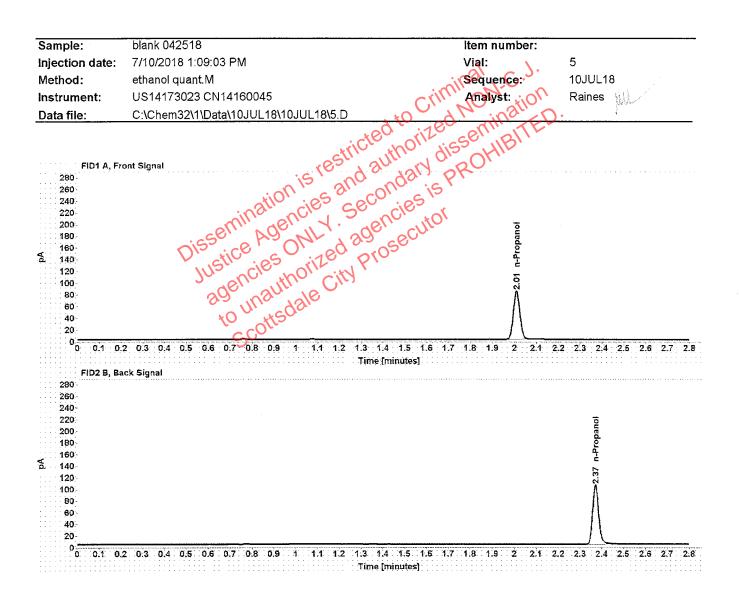


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.010	169.484

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.371	197.593

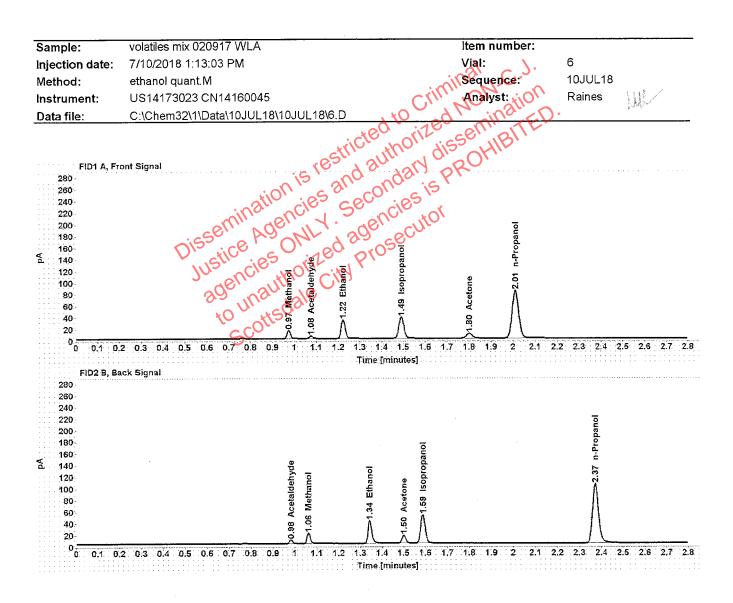


Table 1: FID 1 A (column DB-ALC1)

Methanol 0.974 Acetaldehyde 1.076 >Ethanol 0.0658 1.222 Isopropanol 1.491 Acetone 1.801	Peak Area	Time (min)	Amount (g/100mL)	Compound
>Ethanol	15.903	0.974		Methanol
Isopropanol 1.491	4.840	1.076		Acetaldehyde
toop: oparior	41.279	1.222	0.0658	>Ethanol
Acetone 1.801	59.518	1.491		Isopropanol
	15.003	1.801		Acetone
n-Propanol 2.010	168.432	2.010		n-Propanol

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.982	6.124
Methanol	1.062	19.155
Ethanol	1.343	48.449
Acetone	1.500	17.156
Isopropanol	1.588	71.157
n-Propanol	2.372	196.875

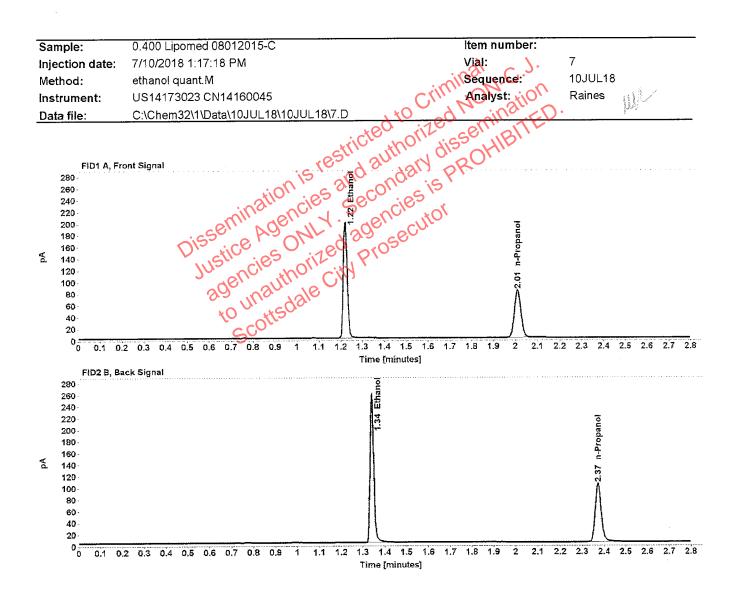


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.3994	1.221	254.138
n-Propanol		2.010	166.673

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.341	304.644
n-Propanol	2.372	195.015

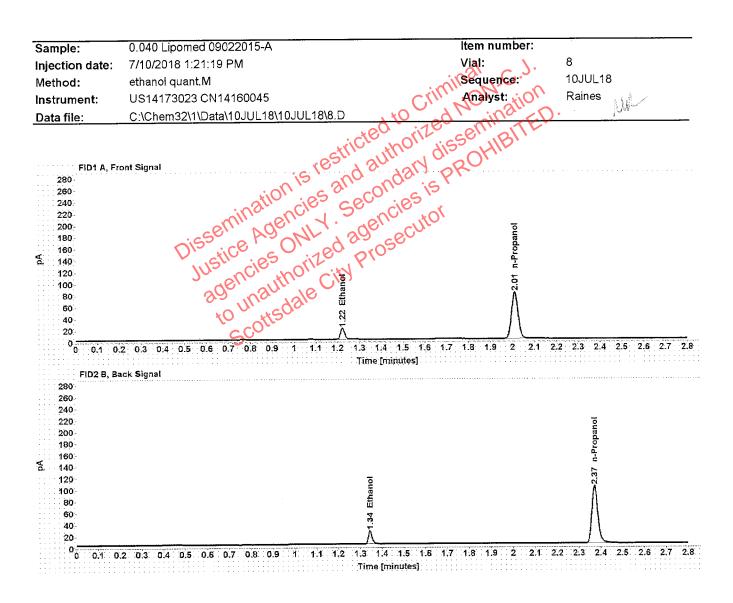


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0407	1.223	24.422
n-Propanol		2.011	164.313

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.344	28.205
n-Propanol	2.372	191.581

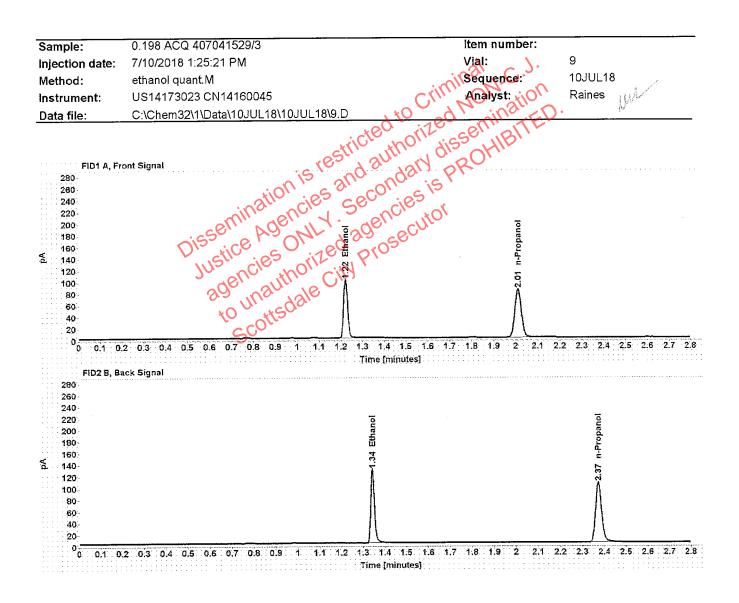


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1980	1.222	128.144
n-Propanol		2.011	170.407

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	152.609
n-Propanol	2.373	199.277

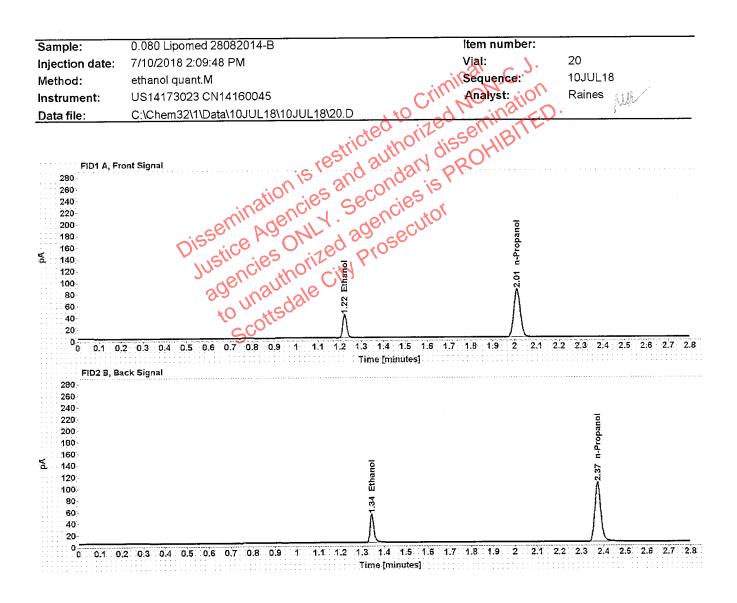


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0809	1.222	51.246
n-Propanol		2.011	169.179

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.343	60.258
n-Propanol	2.373	197.884

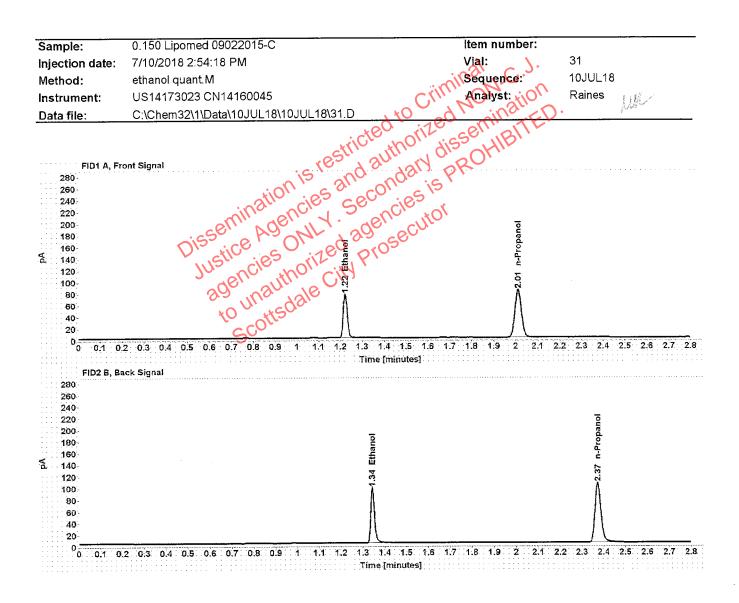


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1523	1.222	97.063
n-Propanol		2.011	168.329

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.343	115.618
n-Propanol	2.373	197.775

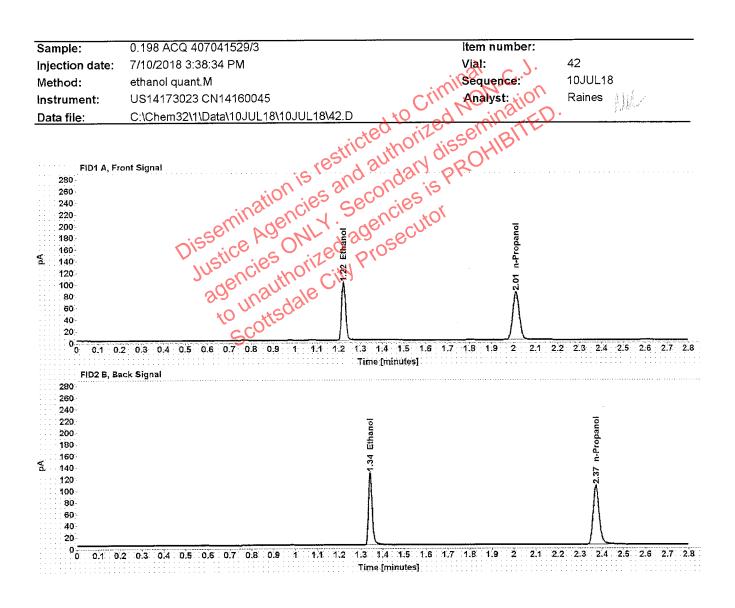


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1989	1.222	126.737
n-Propanol		2.011	167.708

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	151.611
n-Propanol	2.373	197.120

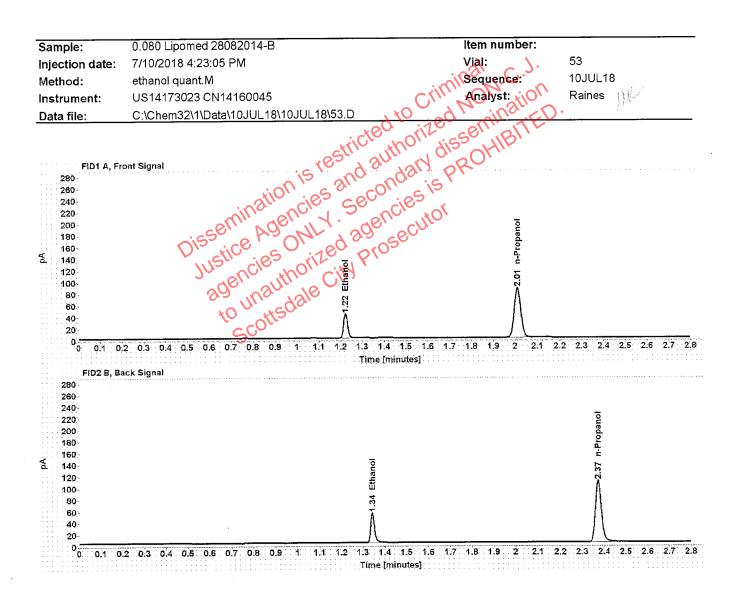


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0819	1.222	53.489
n-Propanol		2.011	174.409

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.343	63.787
n-Propanol	2.373	204.905

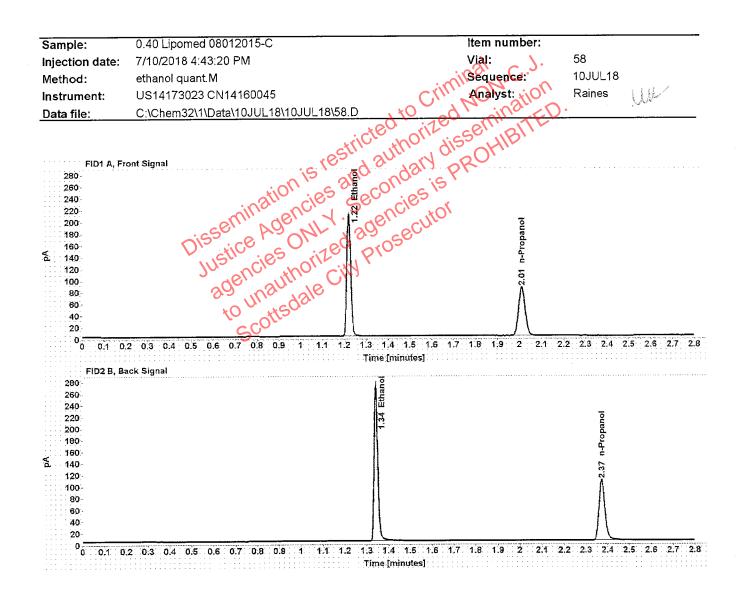


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.4074	1.221	265.605
n-Propanol		2.011	170.762

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	320.817
n-Propanol	2.373	201.391

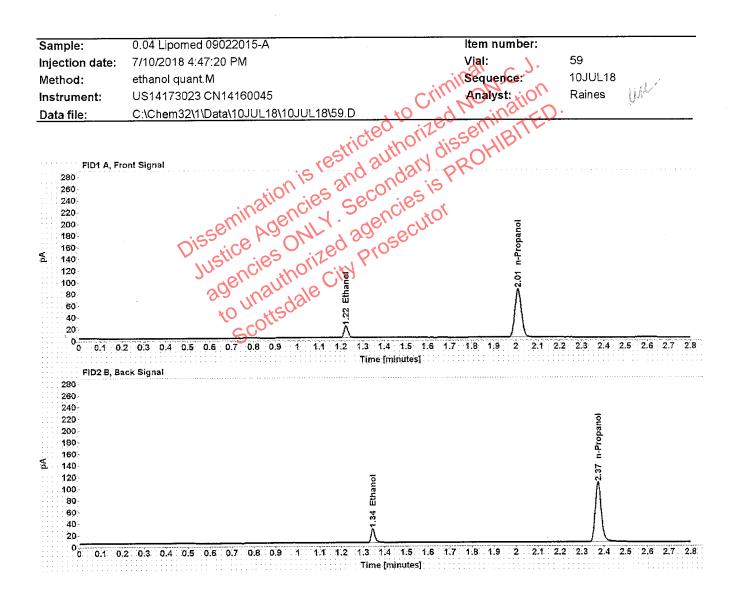


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0412	1.223	25.613
n-Propanol		2.011	169.995

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.344	29.986
n-Propanol	2.373	199.791

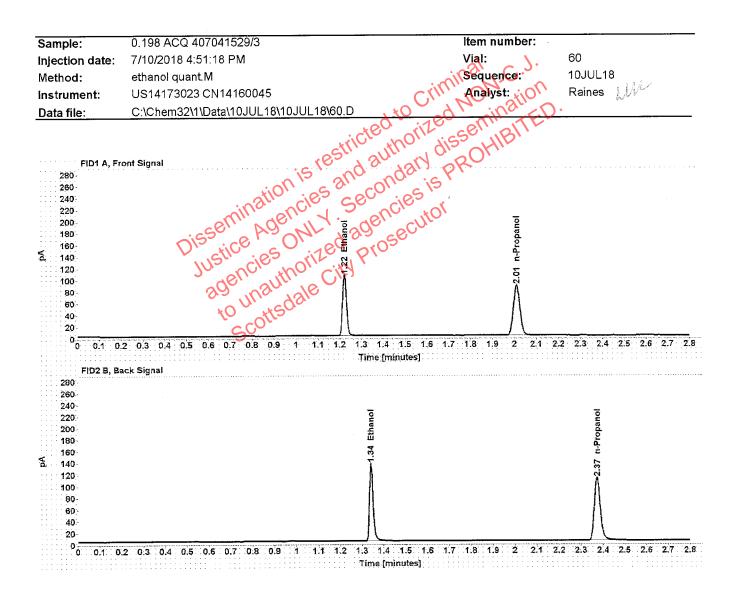


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2006	1.222	134.607
n-Propanol		2.011	176.628

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	161.422
n-Propanol	2.373	207.790

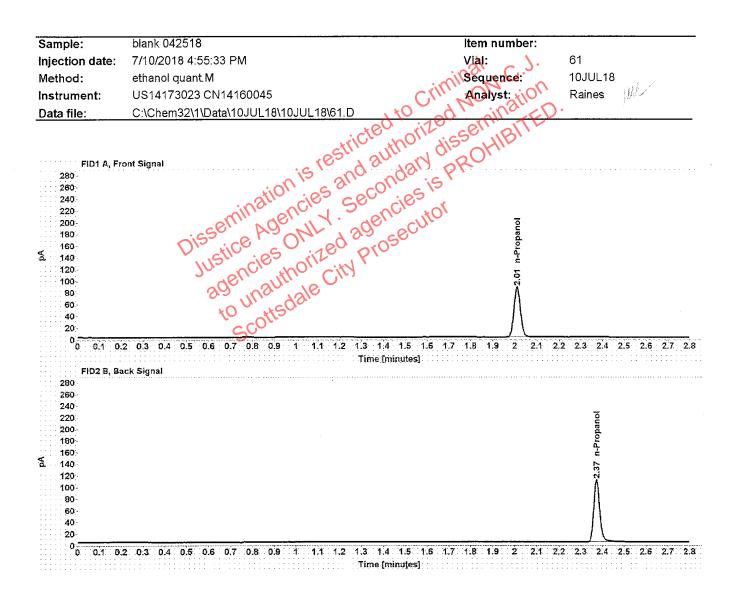


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2,011	175.131

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.373	206.384

Sequence Summary

Page 1 of 2

Analyst: Raines 10JUL18 Instrument: US14173023 CN14160045 Sequence name: Item Number Method Vial Sample Type ethanol quant.M Calibration 0.020 Cerilliant FN03241604 Calibration ethanol quant.M 2 0.100 Cerilliant FN06181501 Calibration ethanol quant.M 0,200 Cerilliant FN07201502 3 0.400 Cerilliant FN11191402 Calibration ethanol quant.M 4 Control ethanol quant.M 5 blank 042518 volatiles mix 020917 WLA Control ethanol quant.M 6 0.400 Lipomed 08012015-C Control ethanol quant.M Control 0.040 Lipomed 09022015-A ethanol quant.M 8 Control ethanol quant.M 9 0.198 ACQ 407041529/3 1212029 ethanol quant.M 10 Sample 1212029 ethanol quant.M Sample 11 312-01A ethanol quant.M Sample 12 312-01A ethanol quant.M 13 Sample Sample 340-01A ethanol quant.M 14 340-01A ethanol quant.M Sample 15 318-02A ethanol quant.M 16 Sample Sample 318-02A ethanol quant.M 17 ethanol quant.M 307-01A Sample 18 307-01A ethanol quant.M 19 Sample 0.080 Lipomed 28082014-B Control ethanol quant.M 20 Sample 1220788 ethanol quant.M 21 1220788 ethanol quant.M 22 Sample Sample 1221001 ethanol quant.M 23 1221001 ethanol quant.M 24 Sample 1222085 ethanol quant.M Sample 25 ethanol quant.M Sample 1222085 26 1222024 ethanol quant.M Sample 27 28 Sample 1222024 ethanol quant.M ethanol quant.M 1222008 29 Sample 1222008 ethanol quant.M Sample 30 ethanol quant.M 31 0.150 Lipomed 09022015-C Control 32 Sample 1221825 ethanol quant.M 1221825 ethanol quant.M Sample 33 Sample 1218383 ethanol quant.M 34 ethanol quant.M 35 Sample 1218383 1217365 ethanol quant.M 36 Sample 1217365 ethanol quant.M Sample 37 1218419 ethanol quant.M Sample 38 39 Sample 1218419 ethanol quant.M 1222978 ethanol quant.M Sample 40 1222978 ethanol quant.M Sample 41 0.198 ACQ 407041529/3 ethanol quant.M Control 42 ethanol quant.M Sample 1202005 43 1202005 ethanol quant.M 44 Sample Sample 1192055 ethanol quant.M 45 ethanol quant.M Sample 1192055 46 1198084 ethanol quant.M 47 Sample

Sequence Summary

	The hard Market in Mills and Market in the section of the section			
48	en en entre more anne en	Sample	1198084	ethanol quant.M
49		Sample	1220386	ethanol quant.M
50		Sample	1220386	ethanol quant.M
51		Sample_ (\)	1223943	ethanol quant.M
52		Sample	1223943	🕥 , ethanol quant.M
53	0.080 Lipomed 28082014-B	Control 10	" WILL	ethanol quant.M
54		Sample	5 1220567	ethanol quant.M
55	5	Sample	1220567	ethanol quant.M
56	is	Sample	1219755	ethanol quant.M
57	ion as a	OSample	1219755	ethanol quant.M
58	0.40 Lipomed 08012015-C	Control		ethanol quant.M
59	0.04 Lipomed 09022015-A	Control		ethanol quant.M
60	0.198 ACQ 407041529/3	Control		ethanol quant.M
61	blank 042518 (5110); eS	Control		ethanol quant.M
	blank 042518 Justine Scottsdale City Scottsdale Scott			

Page 2 of 2

Scottsdale Police Department Crime Laboratory Summary of Cases

SEQUENCE NAME: 10JUL18

ANALYST: Raines

	DE NAME. 1000E10				
Vials	Test 1 (g/dL)	Test 2 (g/dL)	Mean (g/dL)	Percent Difference*	Absolute Difference (g/dL)*
10 11	0.1042	0.1041	0.10415	0.05, 3	0.00005
12 13	0.2145	0.2139	0.21420	0.14	0.00030
14 15	0.1937	0.1938	0.19375	0.03/10	0.00005
16 17	0.1370	0.1371	0.13705	0.04	0.00005
18 19	0.2248	0.2261	0.22545	0.29	0.00065
21 22	0.3142	0.3155	0.31485	0.27	0.00065
23 24	0.1936	0.1945	0.19405	0.23	0.00045
25 26	0.2441	0.2438	0.24395	0.06	0.00015
27 28	0.0482	0(0485	0.04835	0.31	0.00015
29 30	0.0497	0.04970	0.04970	0.00	0.00000
32 33	0.1377	Q.(1370 1	0.13735	0.25	0.00035
34 35	0.1639	0.1644	0.16415	0.15	0.00025
36 37	0.17725	0.1745	0.17585	0.77	0.00135
38 39	0.1852	- 60.1849 1	0.18505	0.08	0.00015
40 41	0.1674	0,1669	0.16715	0.15	0.00025
43 44	0.1616	0.1622	0.16190	0.19	0.00030
45 46	0.0986	0.0980	0.09830	0.31	0.00030
47 48	0.1126	9.1 098	0.11120	1.26	0.00140
49 50	0.1934	0.1949	0.19415	0.39	0.00075
51 52	0.0000	0.0000	0.00000	0.00	0.00000
54 55	0.1339	0.1346	0.13425	0.26	0.00035
56 57	0.2153	0.2180	0.21665	0.62	0.00135

^{*}Calculated differences are differences from the mean of the two results.

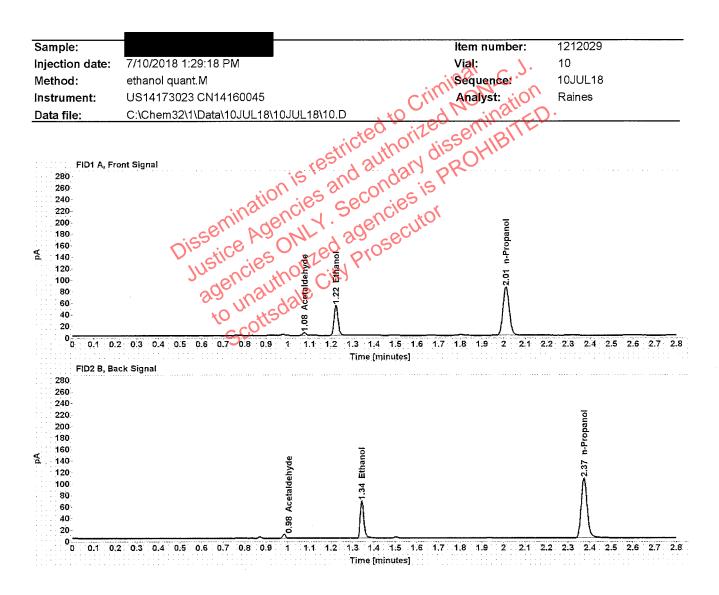


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.309
>Ethanol	0.1042	1.222	67.325
n-Propanol		2.011	171.633

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.690
Ethanol	1.343	79.093
n-Propanol	2.373	201.221

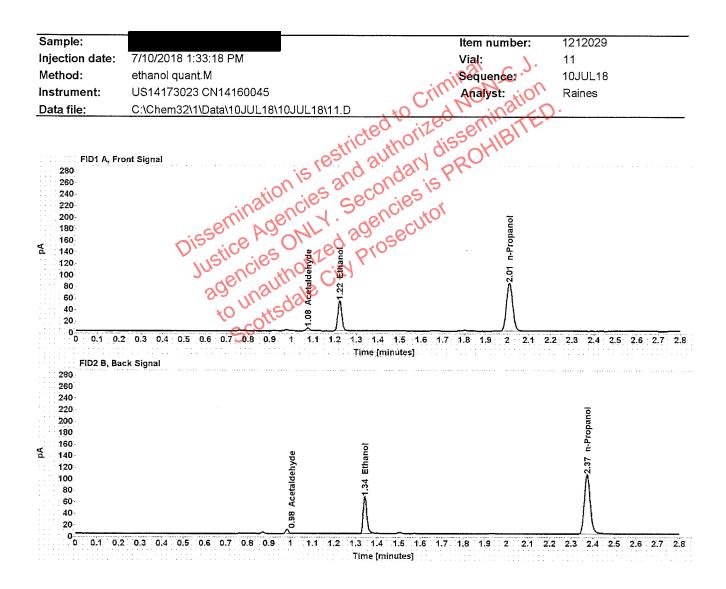


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.492
>Ethanol	0.1041	1.222	66.827
n-Propanol		2.011	170.463

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.957
Ethanol	1.343	78.462
n-Propanol	2.373	200.064

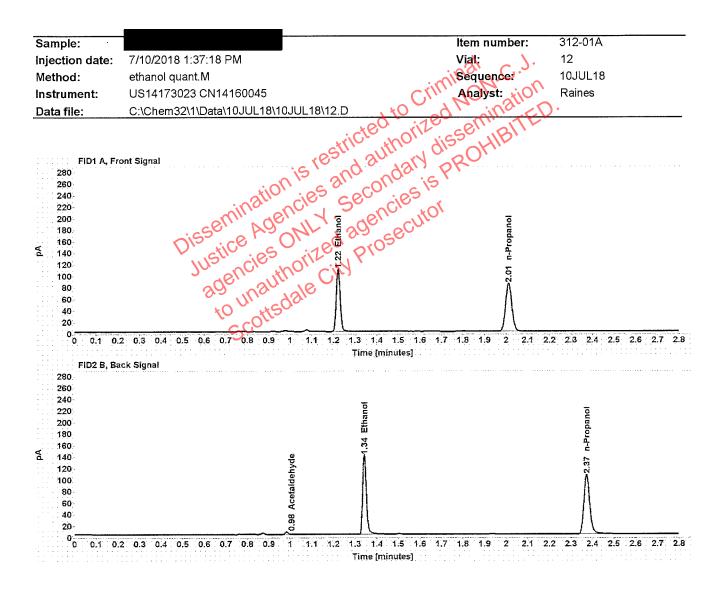


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2145	1.222	138.952
n-Propanol		2.011	170.436

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	4.212
Ethanol	1.342	165.373
n-Propanol	2.373	200.278

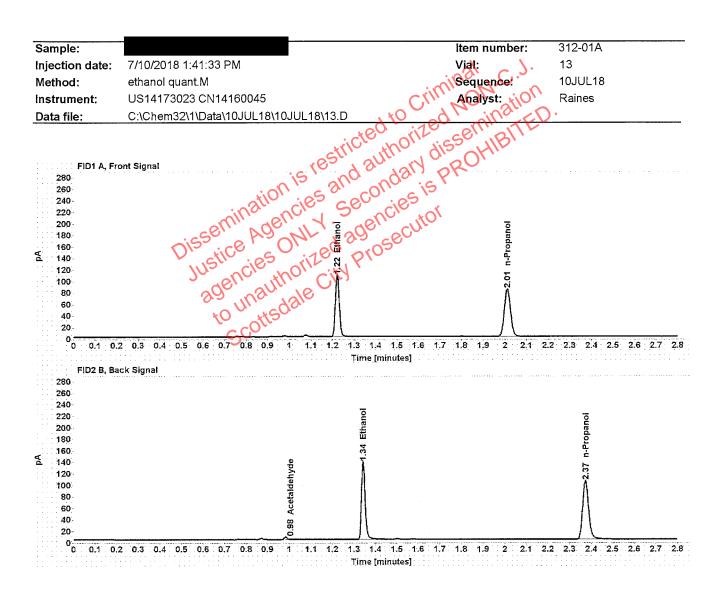


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2139	1,222	136.676
n-Propanol		2.011	168.120

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	4.197
Ethanol	1.342	162.706
n-Propanol	2.373	197.627

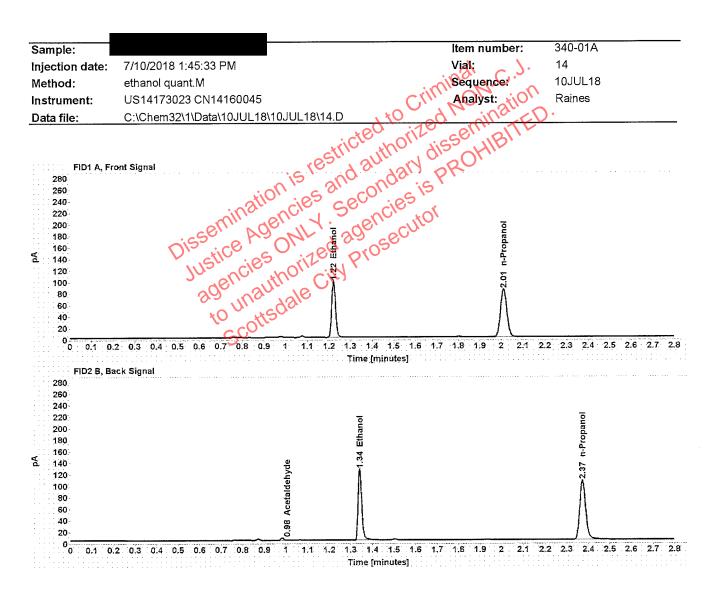


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1937	1.222	125.024
n-Propanol		2.011	169.985

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	3.774
Ethanol	1.342	148.206
n-Propanol	2.372	199.786

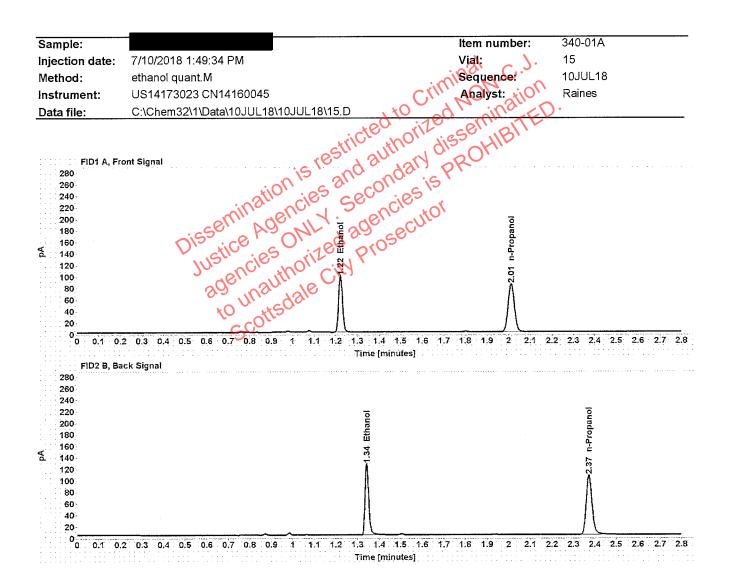


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1938	1.222	125.037
n-Propanol		2.011	169.878

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	148.243
n-Propanol	2.372	199.861

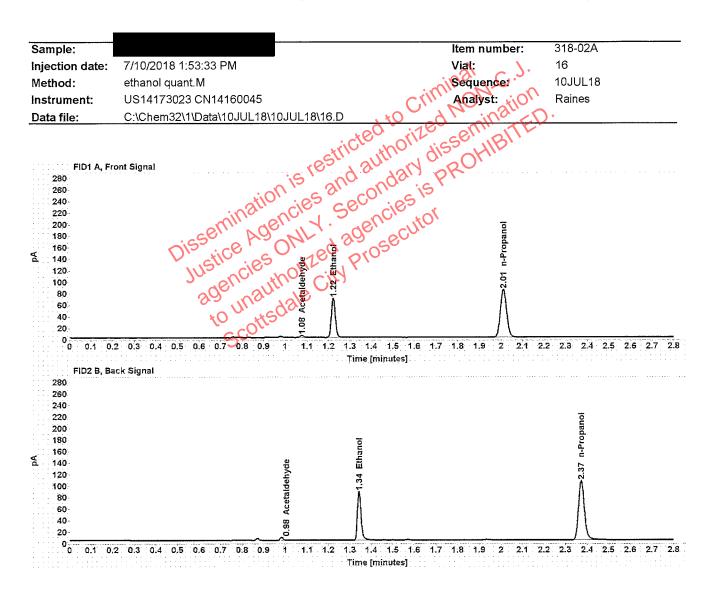


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	3.988
>Ethanol	0.1370	1.222	87.691
n-Propanol		2.011	169.263

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.054
Ethanol	1.342	103.366
n-Propanol	2.373	199.143

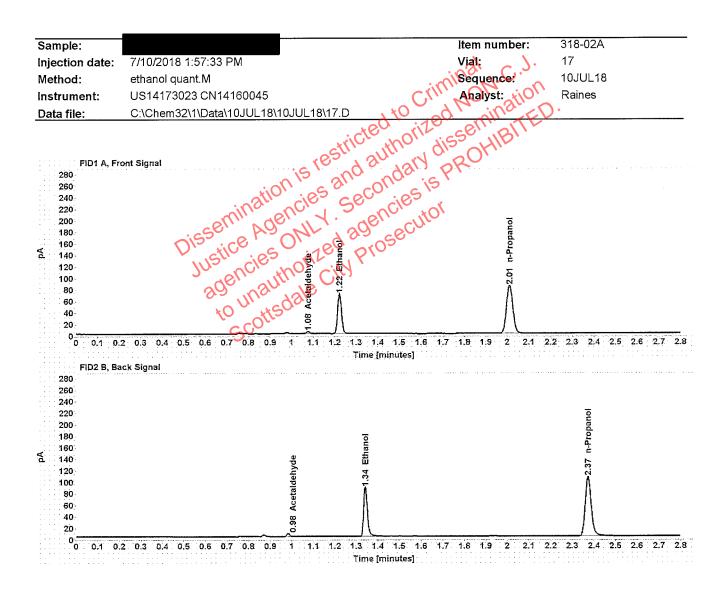


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaidehyde		1.076	3.979
>Ethanoi	0.1371	1.222	88.160
n-Propanol		2.011	170.101

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.028
Ethanol	1.342	104.018
n-Propanol	2.372	200.189

User: mraines 7/11/2018

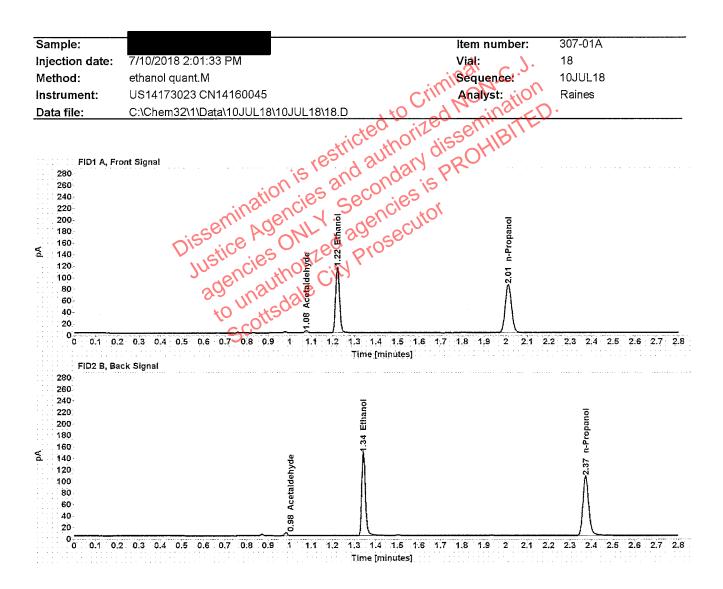


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.080
>Ethanol	0.2248	1.222	145.621
n-Propanol		2.011	170.356

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.175
Ethanol	1.342	173.571
n-Propanol	2.373	200.094

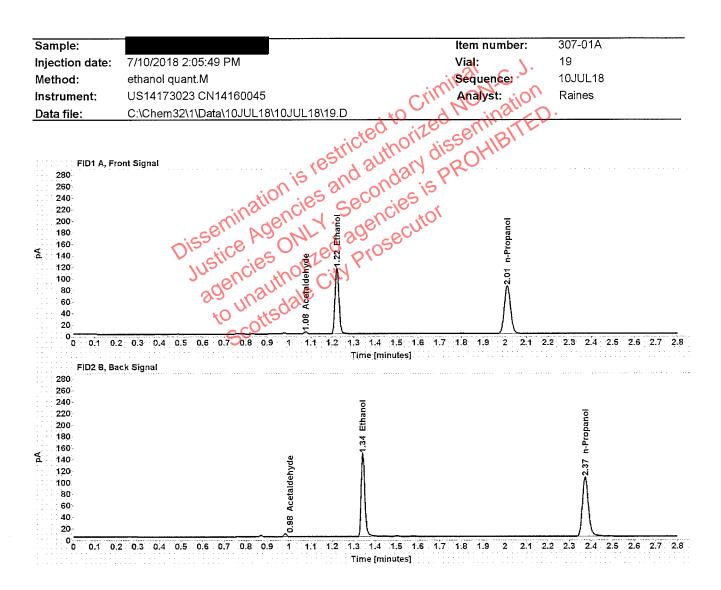


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.102
>Ethanol	0.2261	1.222	146.274
n-Propanol	20000	2.011	170.072

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.178
Ethanol	1.342	173.867
n-Propanol	2.373	200.053

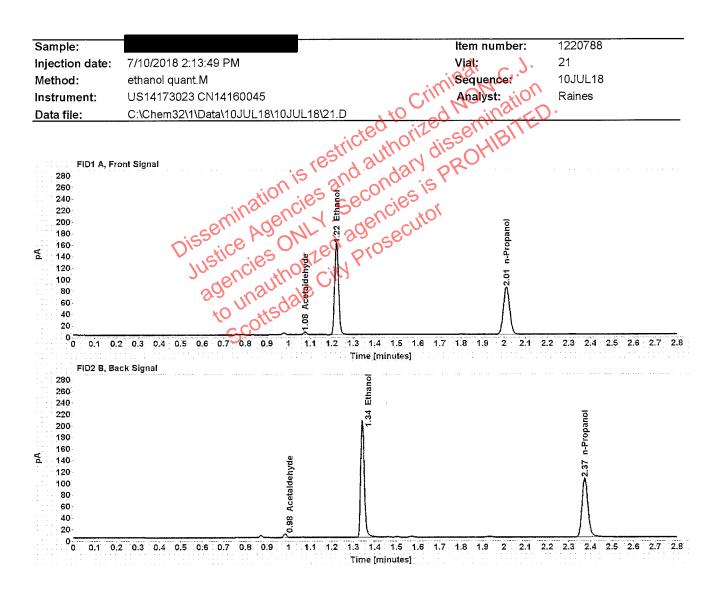


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.877
>Ethanol	0.3142	1.222	203.210
n-Propanol		2.011	169.628

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.126
Ethanol	1.342	244.230
n-Propanol	2.373	196.026

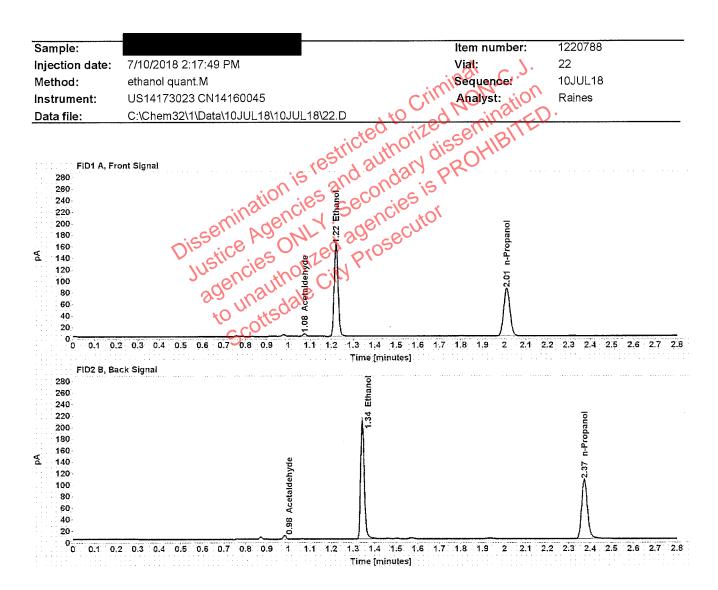


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.879
>Ethanol	0.3155	1.222	205.177
n-Propanol		2.011	170.562

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.159
Ethanol	1.342	246.809
n-Propanol	2.373	197.558

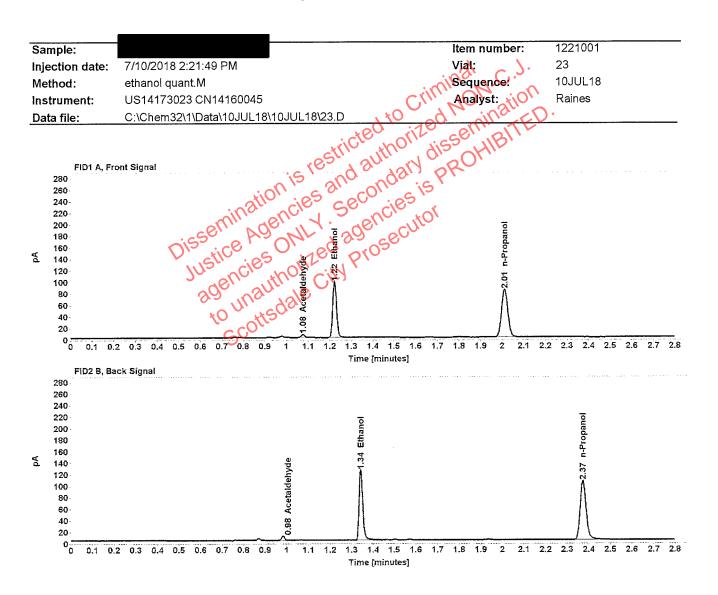


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.779
>Ethanol	0.1936	1.222	123.701
n-Propanol		2.011	168.237

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	7.277
Ethanol	1.342	148.603
n-Propanol	2.373	198.507

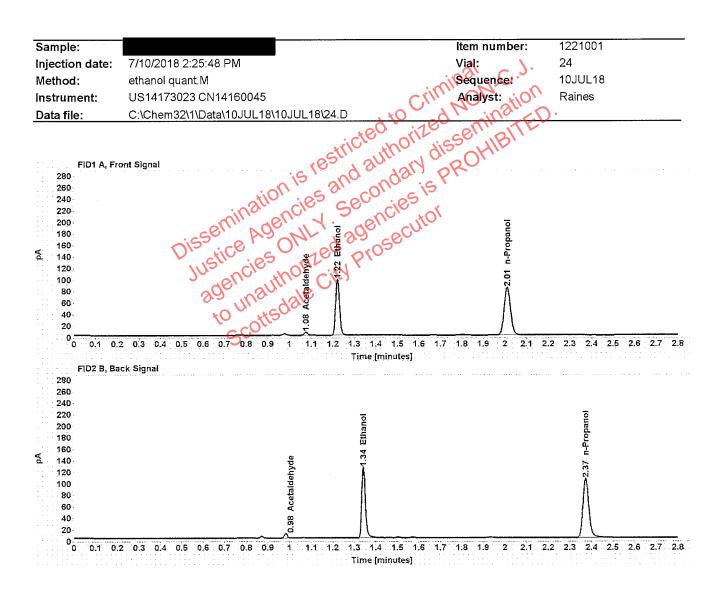


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde	***	1.076	5.851
>Ethanol	0.1945	1.222	124.504
n-Propanol		2.011	168.553

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	7.363
Ethanol	1.342	149.538
n-Propanol	2.372	199.051

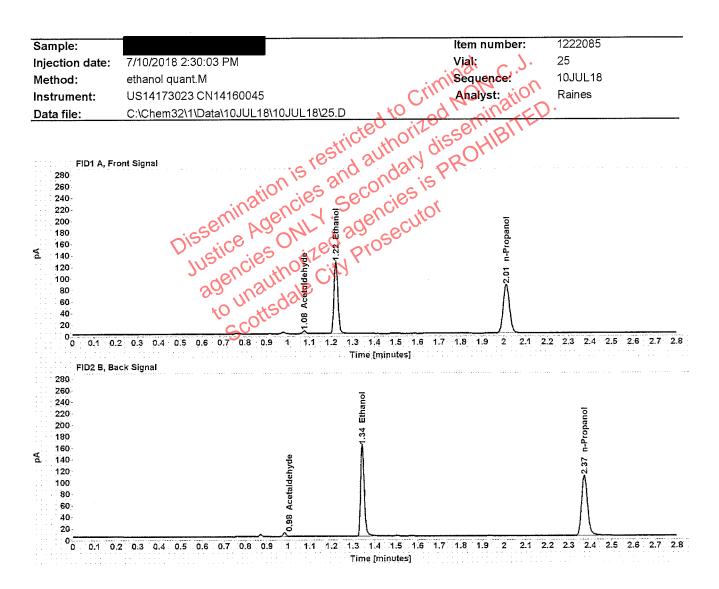


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.046
>Ethanol	0.2441	1.222	159.632
n-Propanol		2.011	171.811

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.400
Ethanol	1.342	191.575
n-Propanol	2.373	203.015

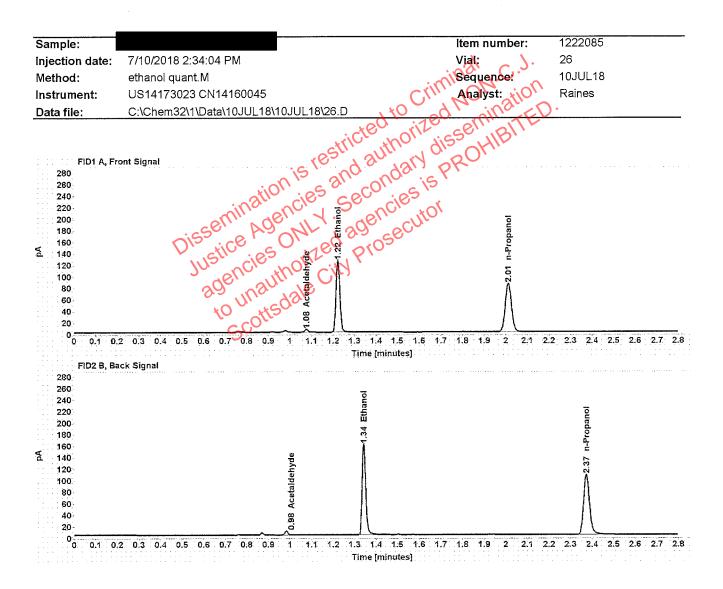


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.079
>Ethanol	0.2438	1.222	158.987
n-Propanol		2.011	171.328

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.400
Ethanol	1.342	190.930
n-Propanol	2.373	202.342

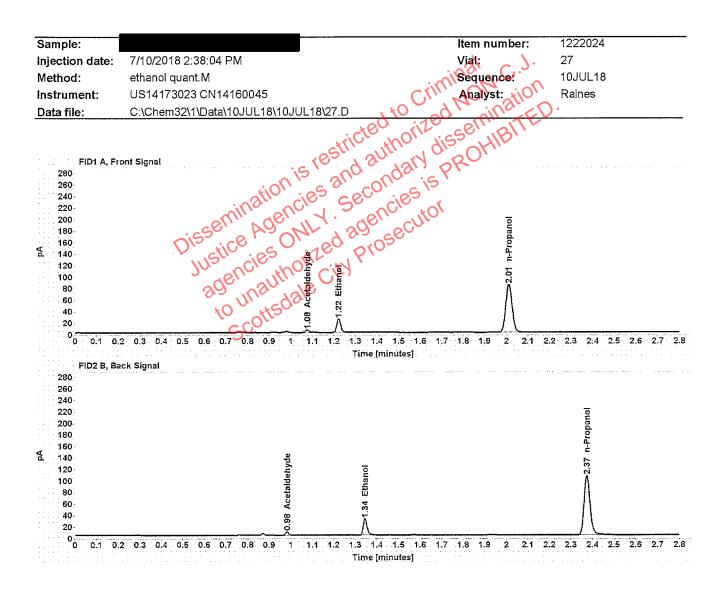


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.600
>Ethanol	0.0482	1.223	30,063
n-Propanol		2.011	169.658

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5,825
Ethanol	1.344	35.703
n-Propanol	2.373	200.032

User: mraines 7/11/2018

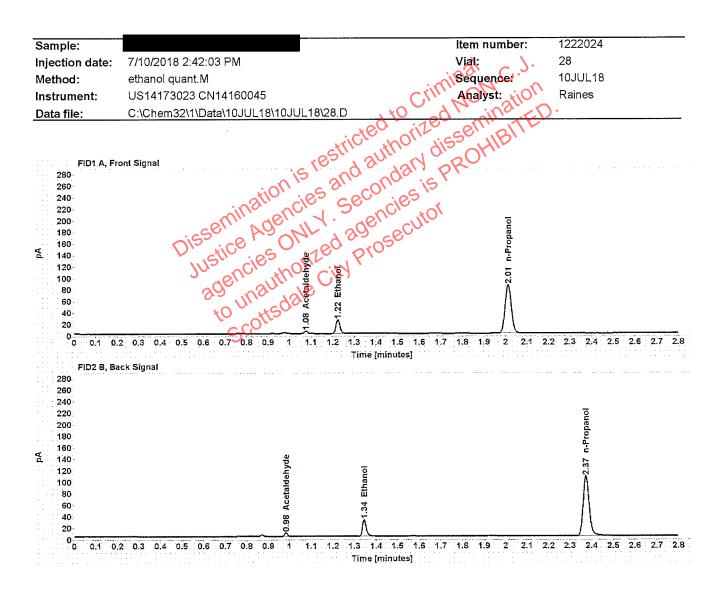


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.602
>Ethanol	0,0485	1.223	30.472
n-Propanol		2.012	170.751

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.755
Ethanol	1.345	36,290
n-Propanol	2.374	201.276

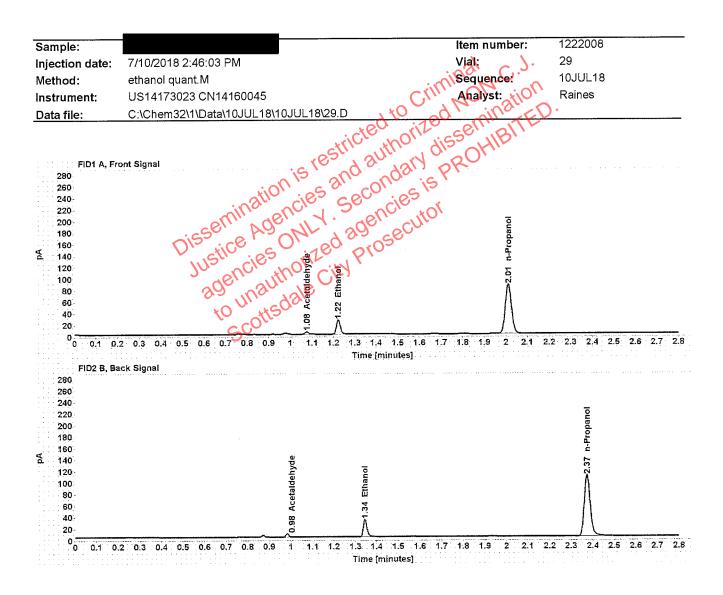


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.281
>Ethanol	0.0497	1.223	31.890
n-Propanol		2.011	174.125

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.391
Ethanol	1.344	37.981
n-Propanol	2.373	205.192

Jser: mraines 7/11/2018

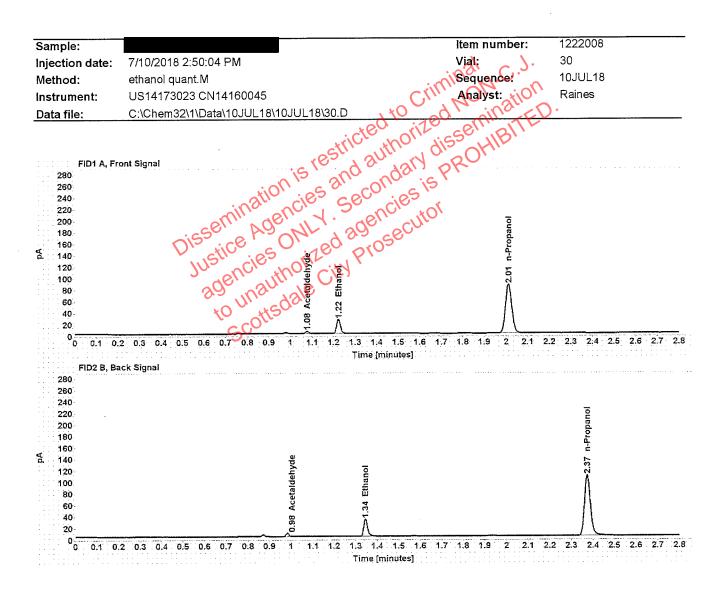


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.295
>Ethanol	0.0497	1.223	31.711
n-Propanol		2.011	173.125

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.397
Ethanol	1.345	37.757
n-Propanol	2.373	204.091

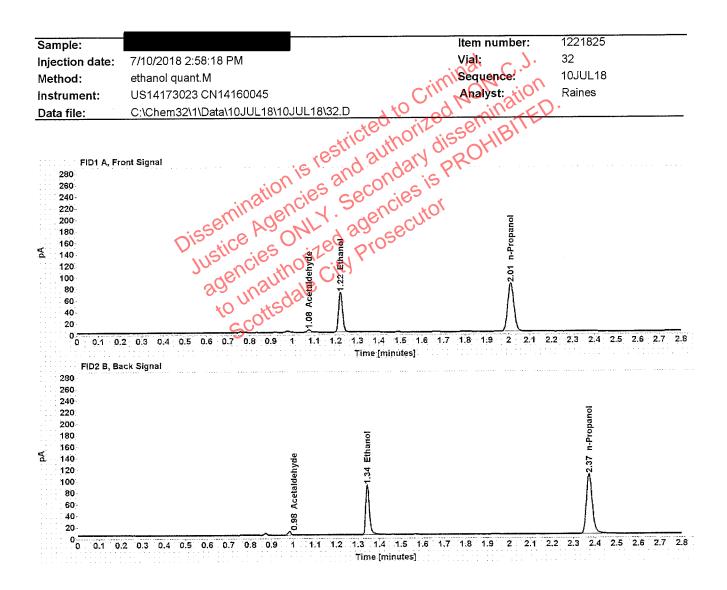


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.656
>Ethanol	0.1377	1.222	88.816
n-Propanol		2.011	170.506

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.859
Ethanol	1.343	104.907
n-Propanol	2.373	201.364

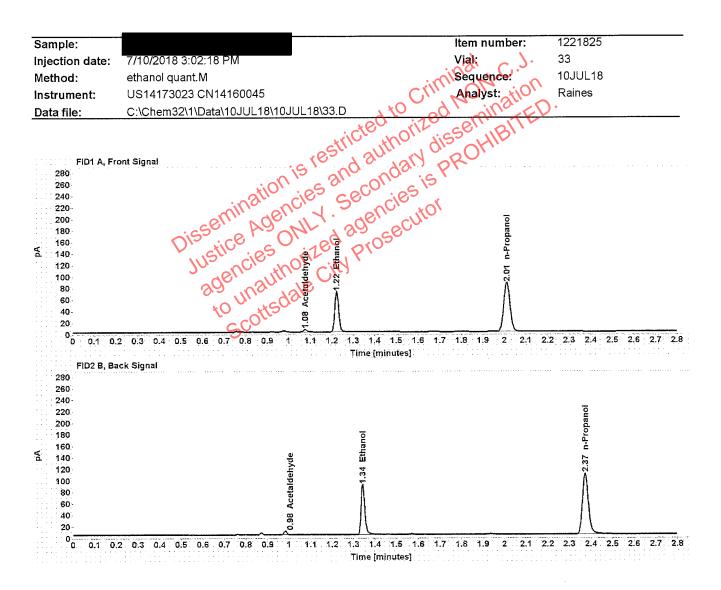


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.725
>Ethanol	0.1370	1.222	89.742
n-Propanol		2.011	173.226

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.978
Ethanol	1.343	106.029
n-Propanol	2.373	204.813

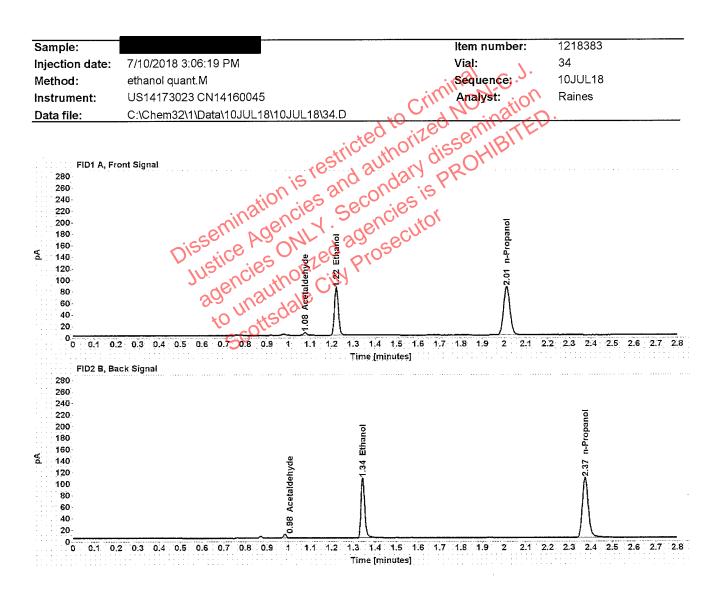


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.963
>Ethanol	0.1639	1.222	106.560
n-Propanol		2.011	171.529

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.263
Ethanol	1.342	126.440
n-Propanol	2.373	202.274

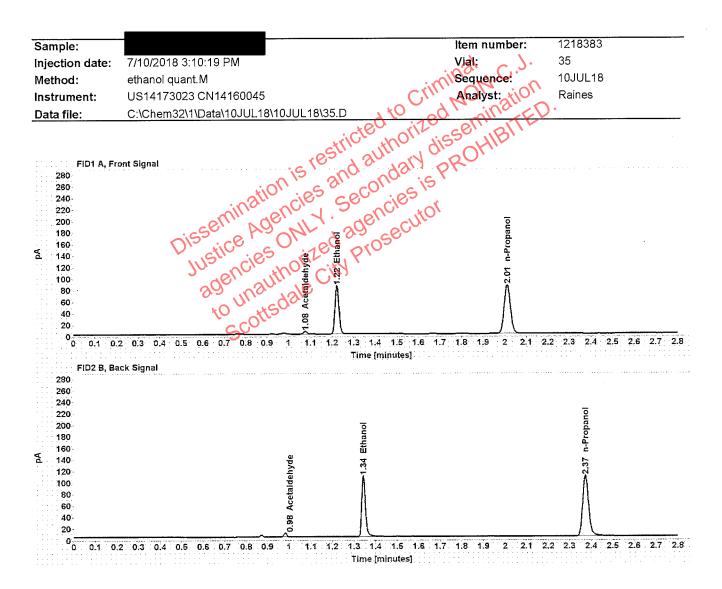


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.054
>Ethanol	0.1644	1.222	107.843
n-Propanol		2.011	173.017

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.360
Ethanol	1.343	127.626
n-Propanol	2.373	204.049

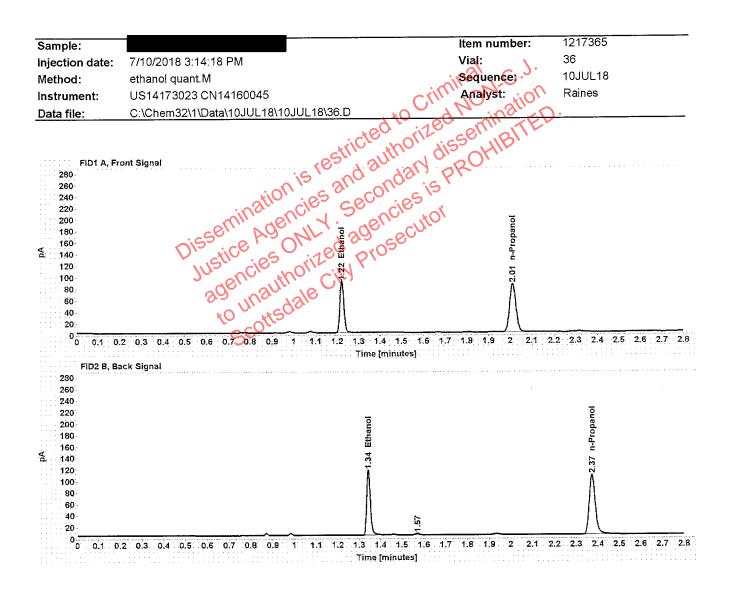


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1772	1.222	115.501
n-Propanol		2.011	171.824

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	139.145
n-Propanol	2.373	201.534

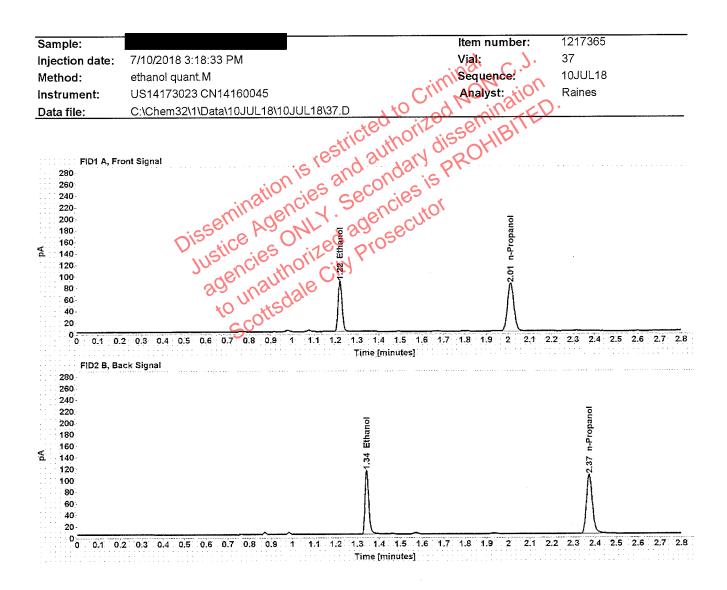


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1745	1.222	112.769
n-Propanol	******	2.011	170.379

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	135.573
n-Propanol	2.373	199.913

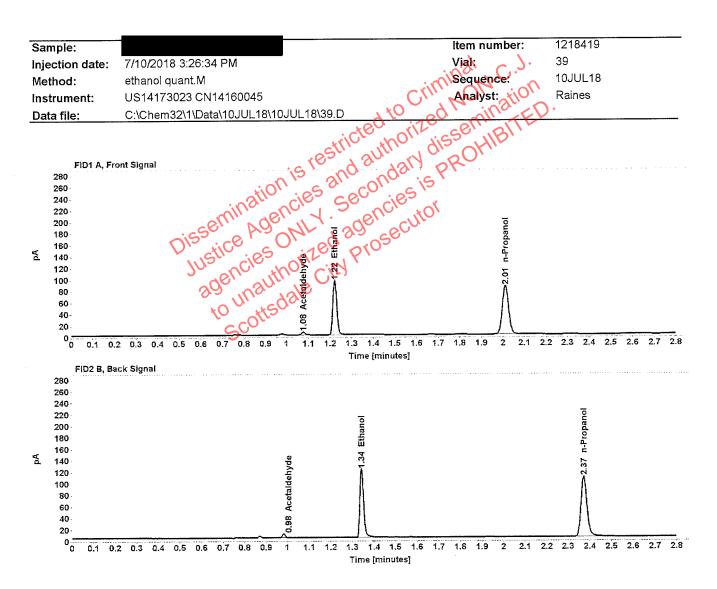


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.997
>Ethanol	0.1849	1.222	120.564
n-Propanol		2.011	171.752

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.294
Ethanol	1.342	143.427
n-Propanol	2.373	202.469

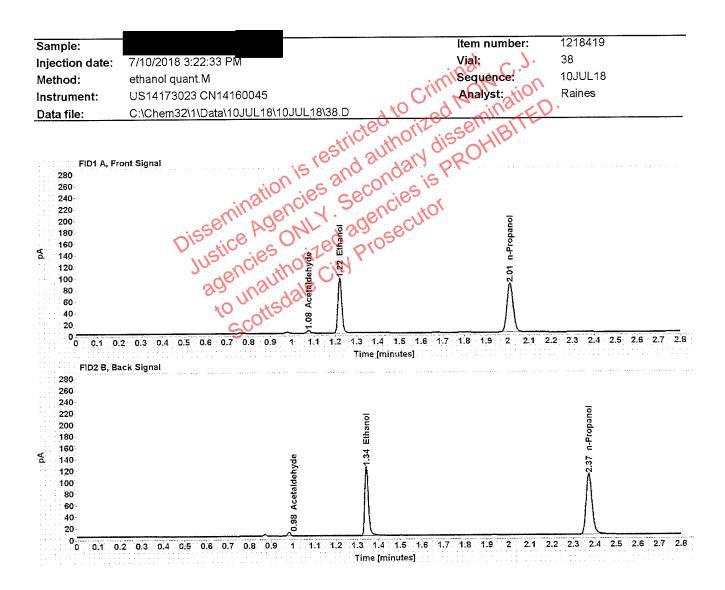


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaidehyde		1.076	4.986
>Ethanol	0.1852	1.222	121.824
n-Propanol		2.011	173.262

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.270
Ethanol	1.342	144.749
n-Propanol	2.373	204.566

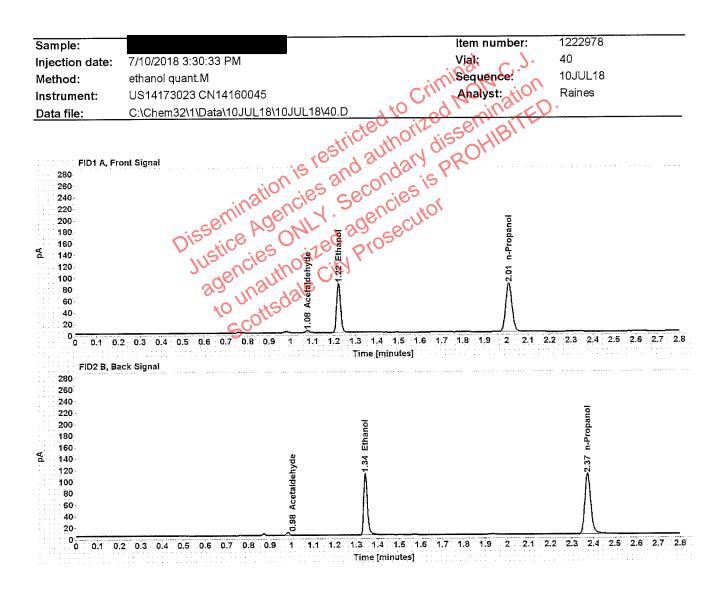


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	3.961
>Ethanol	0.1674	1.222	109.146
n-Propanol		2.011	171.955

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.027
Ethanol	1.342	131.343
n-Propanol	2.373	203.735

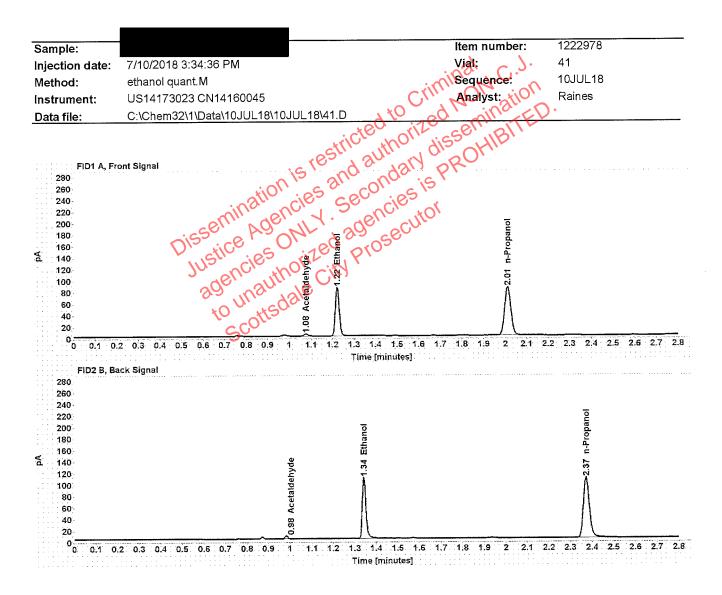


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.026
>Ethanol	0.1669	1.222	108.308
n-Propanol		2.011	171.170

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.095
Ethanol	1.342	130.166
n-Propanol	2.373	202.600

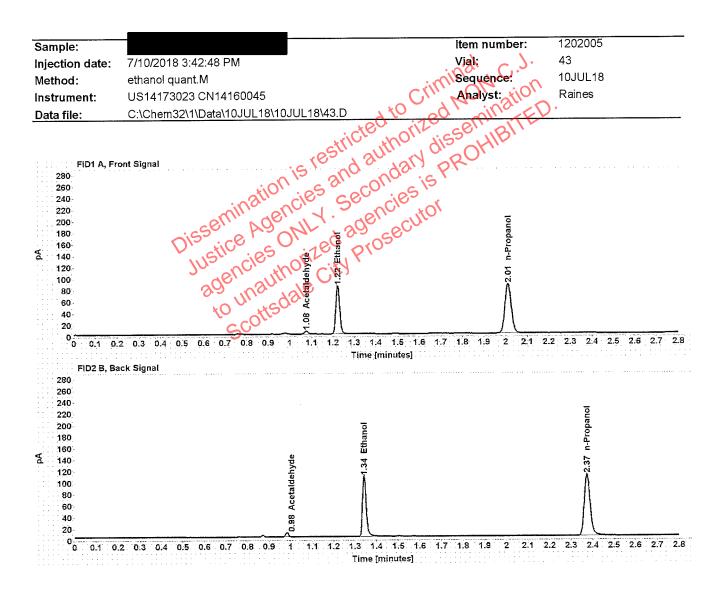


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.550
>Ethanol	0,1616	1.222	107.302
n-Propanol		2.011	175.200

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.935
Ethanol	1.343	127.830
n-Propanol	2.374	206.692

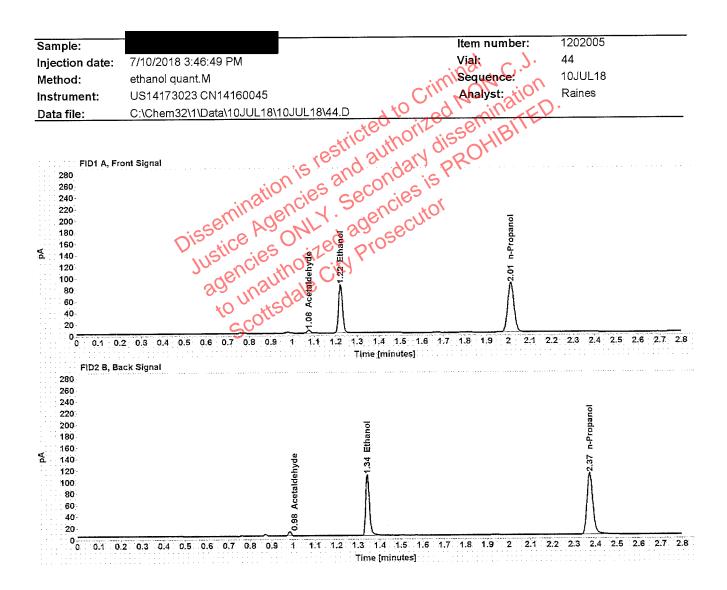


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.606
>Ethanol	0.1622	1.222	107.754
n-Propanol		2.011	175.315

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	7.023
Ethanol	1.342	128.448
n-Propanol	2.373	206.833

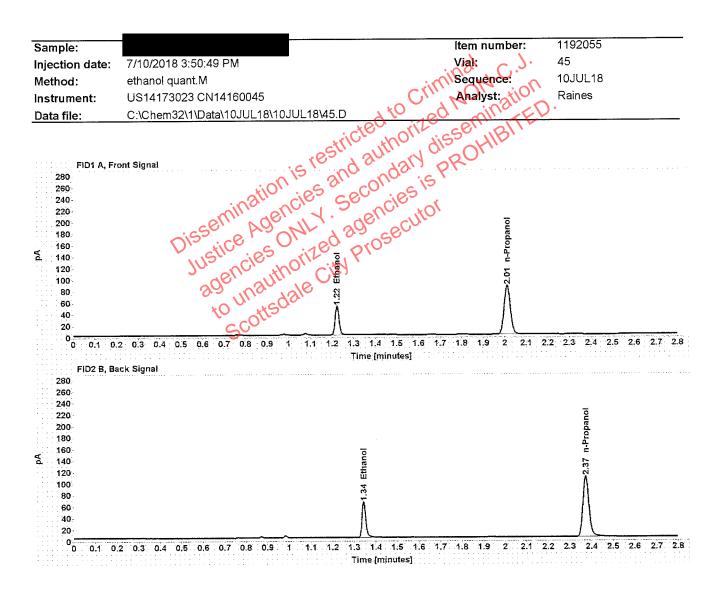


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0986	1.222	64.042
n-Propanol	AL 40 FIRST 199	2.011	172.788

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.343	75.778
n-Propanol	2.373	203.875

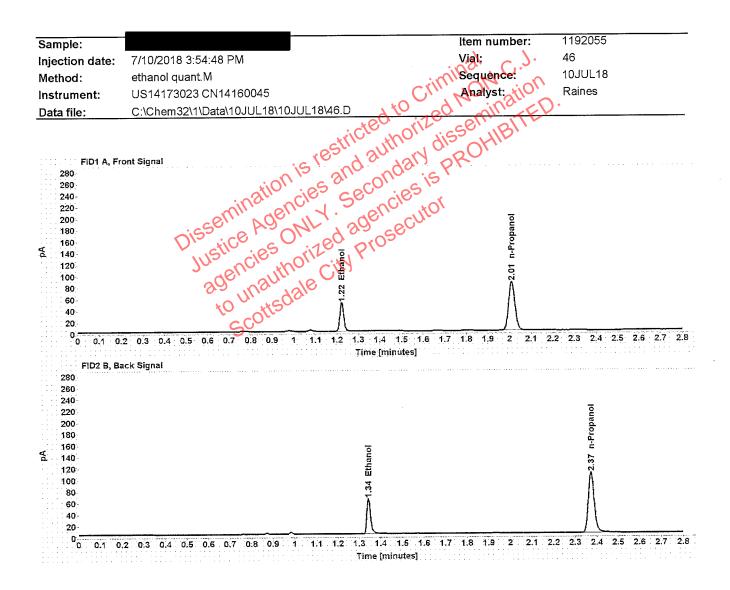


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0980	1.222	63.396
n-Propanol		2.011	172.015

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.343	74.949
n-Propanol	2.373	202.909

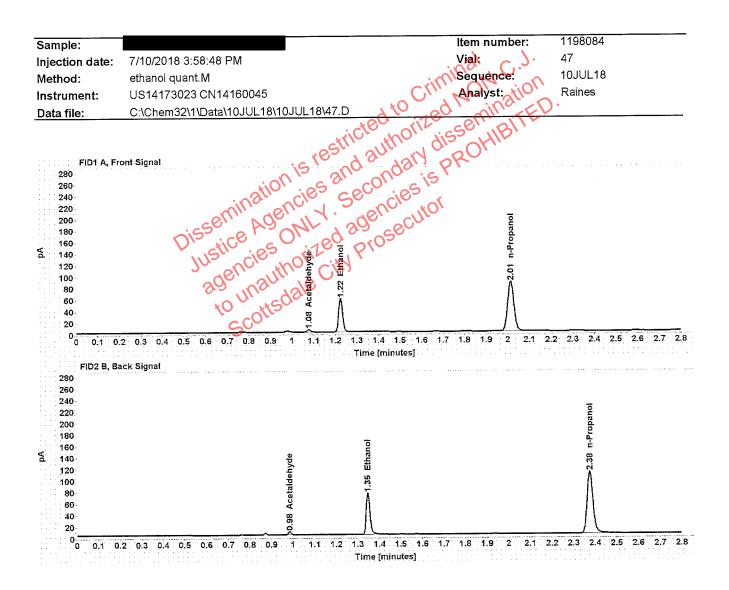


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.077	4.230
>Ethanol	0.1126	1.224	74.568
n-Propanol		2.013	175.659

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.984	5.306
Ethanol	1.346	87.723
n-Propanol	2,375	207.135

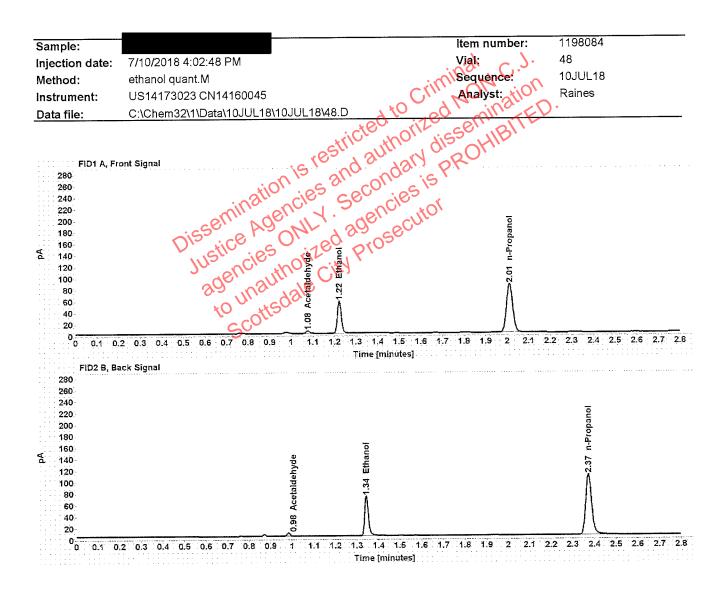


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.344
>Ethanol	0.1098	1.222	71.386
n-Propanol		2.011	172.607

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	5.486
Ethanol	1.343	83.806
n-Propanol	2.373	203.572

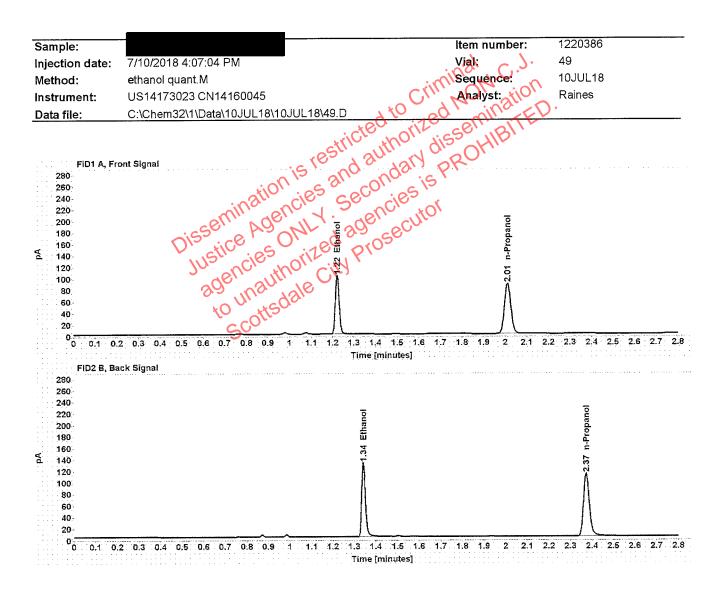


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1934	1.222	130.791
n-Propanol		2.011	178.122

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.342	155.964
n-Propanol	2.373	210,956

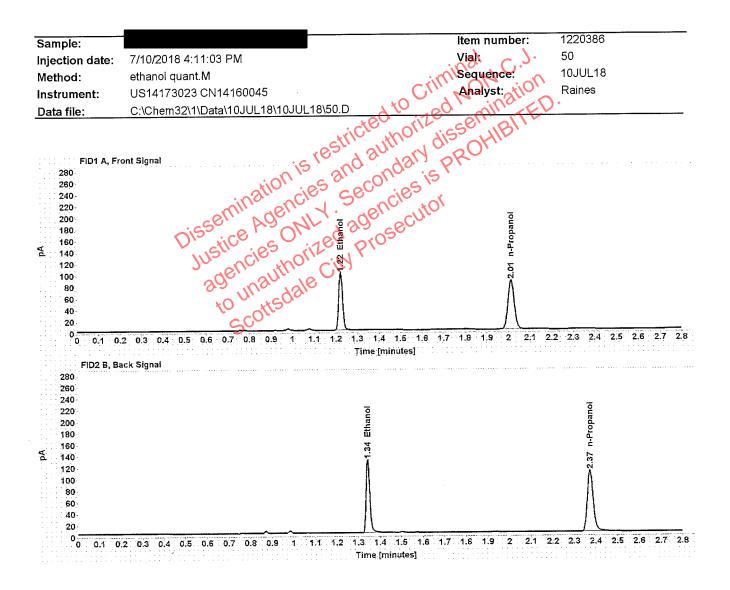


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1949	1.222	128.491
n-Propanol		2.011	173.574

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.343	153.159
n-Propanol	2.373	205.449

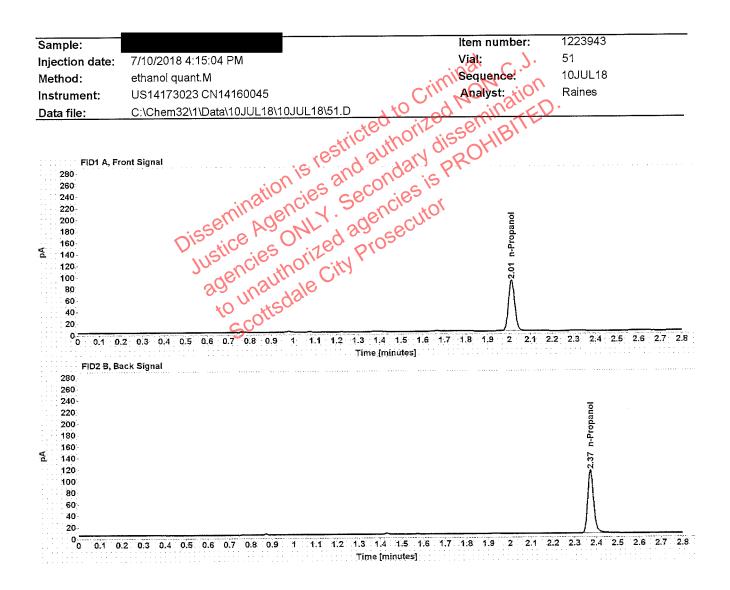


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.011	178.806

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.373	211.387

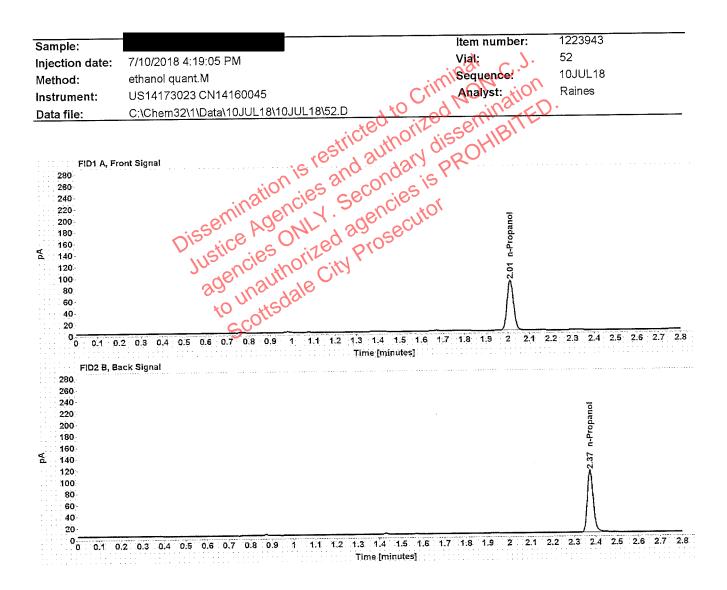


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.012	176.638

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.374	209.023

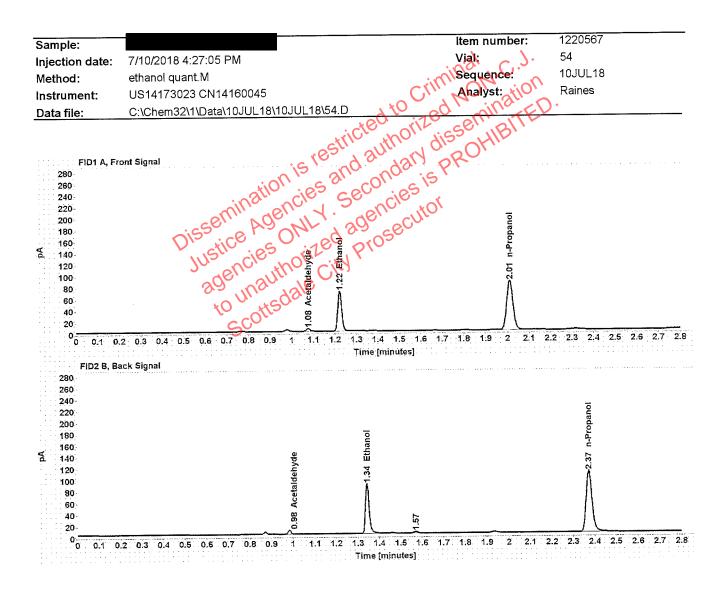


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	5.045
>Ethanol	0.1339	1.222	88.860
n-Propanol		2.011	175.498

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.376
Ethanol	1.342	106.947
n-Propanol	2.373	205.948

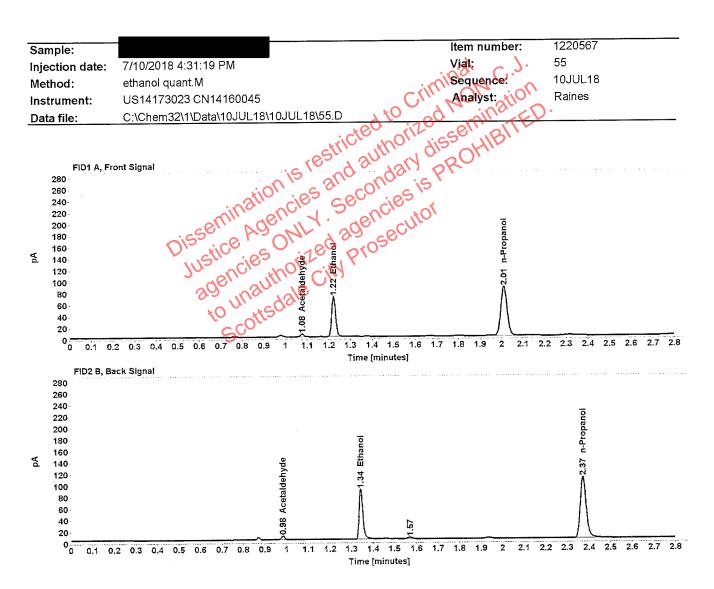


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.076	4.948
>Ethanol	0.1346	1.222	89.210
n-Propanol		2.011	175.287

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	6.298
Ethanol	1.342	107.160
n-Propanol	2.373	205.985

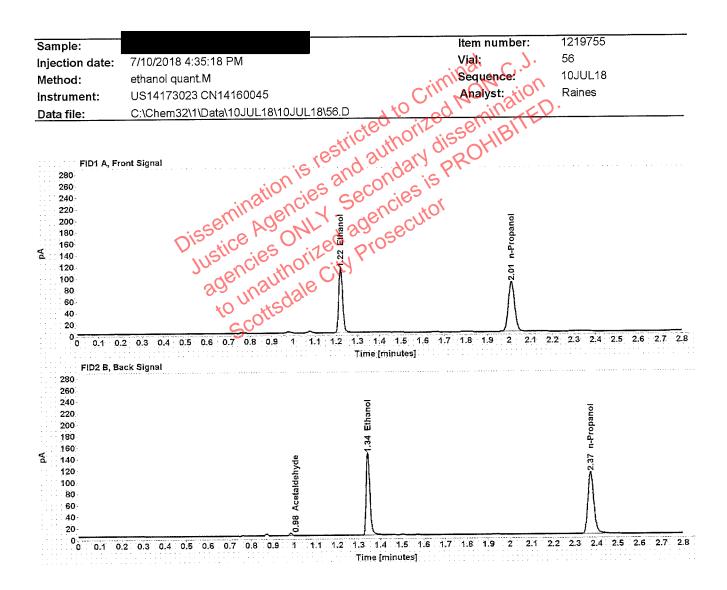


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2153	1.222	143.822
n-Propanol		2.011	175.695

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.983	3.914
Ethanol	1.342	173,540
n-Propanol	2.373	208.505

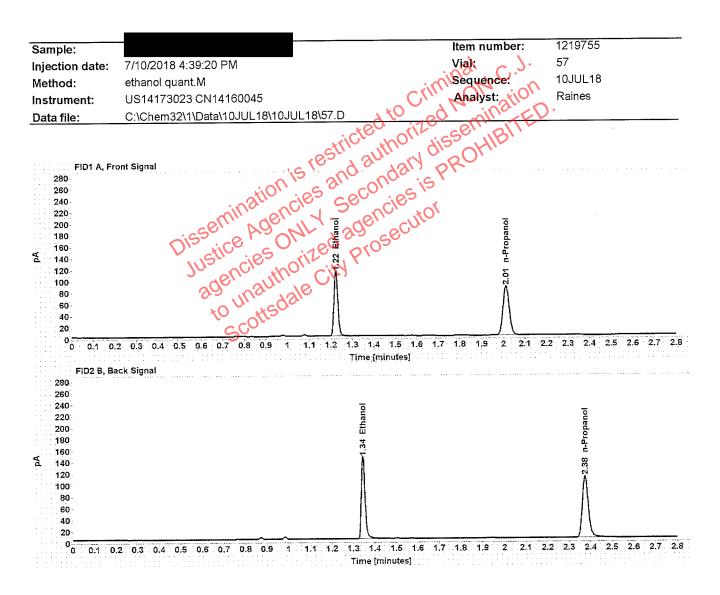


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2180	1.223	144.273
n-Propanol		2.012	174.046

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.344	173.691
n-Propanol	2.375	206.608