User: wadrian 3/18/2019

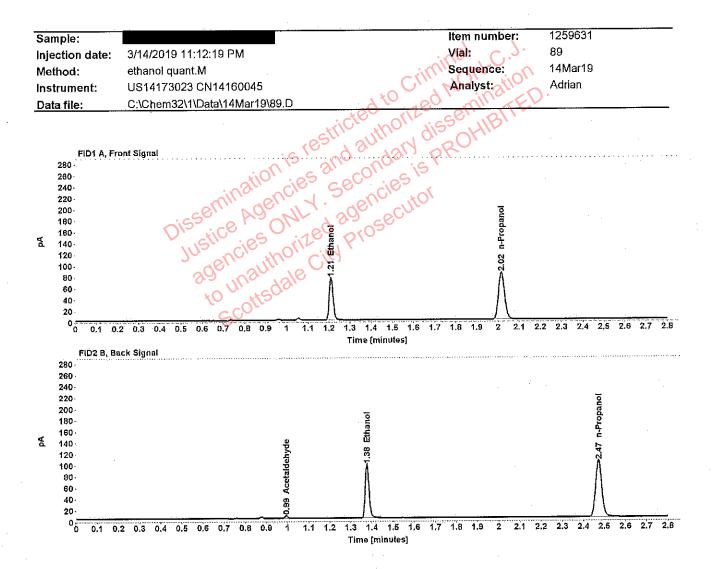


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1526	1.210	96.513
n-Propanol		2.017	167.088

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.697
Ethanol	1.377	120,359
n-Propanol	2.472	205.813

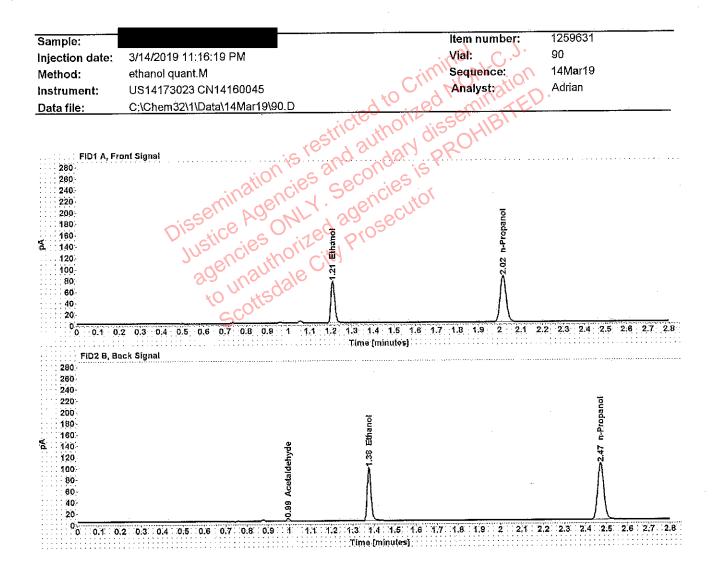


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1518	1.210	95.302
n-Propanol		2.016	165.833

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.757
Ethanol	1.376	118.435
n-Propanol	2,472	204.126

Jser: wadrian 3/18/2019

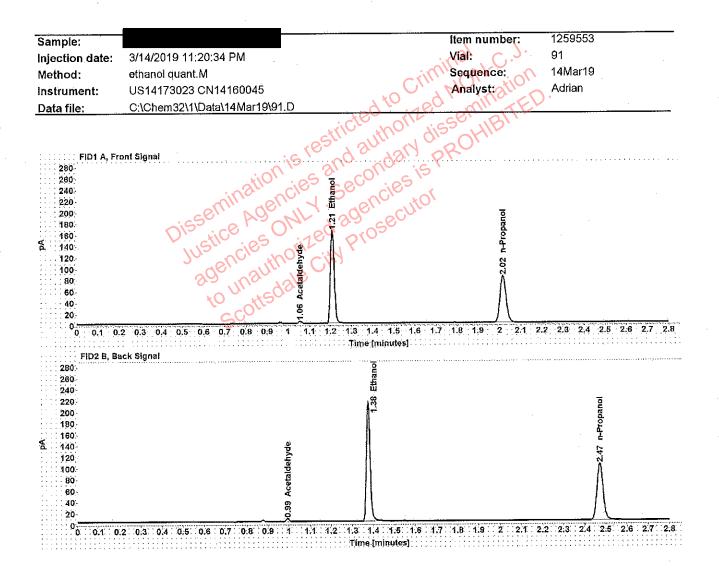


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	3.937
>Ethanol	0.3338	1.209	211.185
n-Propanol		2.016	166,439

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5.170
Ethanol	1.376	263,580
n-Propanol	2.472	204.848

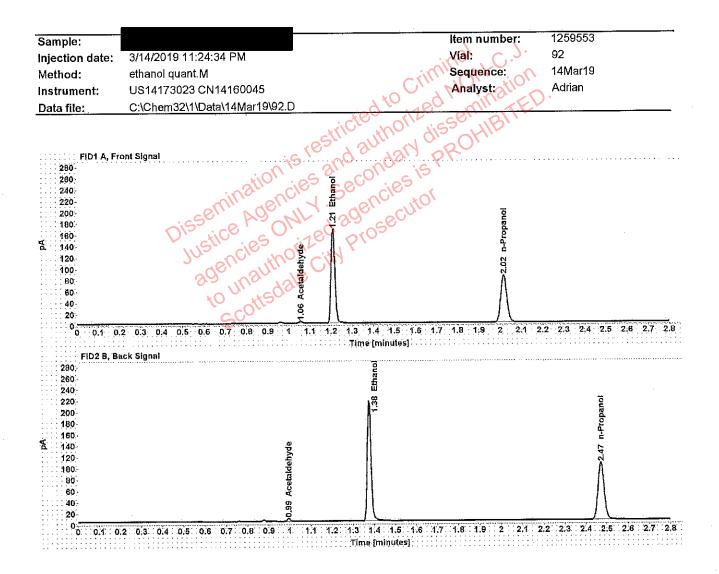


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	3,868
>Ethanol	0.3345	1.209	213.547
n-Propanol		2.016	167.926

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5,106
Ethanol	1.376	266.499
n-Propanol	2.472	206.871

User: wadrian 3/18/2019

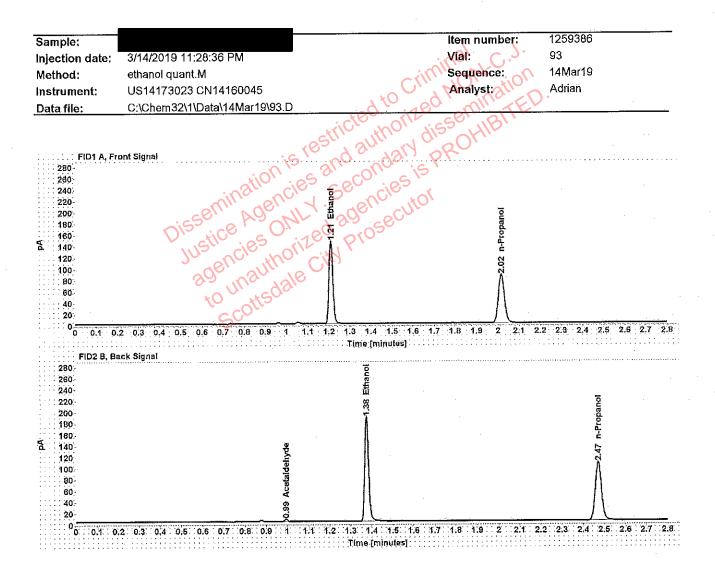


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2856	1.209	186.990
n-Propanol		2.016	172,363

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	3.954
Ethanol	1.376	233.358
n-Propanol	2,472	212.004

Jser: wadrian 3/18/2019

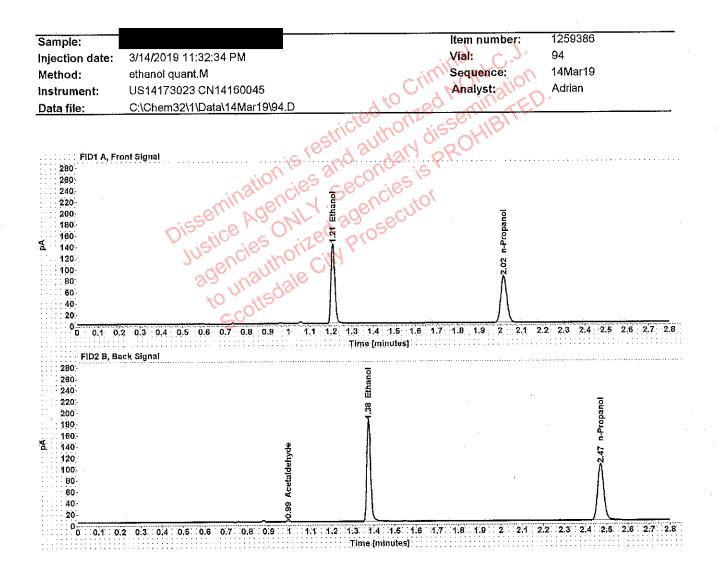


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2867	1.209	180.998
n-Propanol	=	2.016	166.185

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.000
Ethanol	1,375	226.265
n-Propanol	2.471	204.257

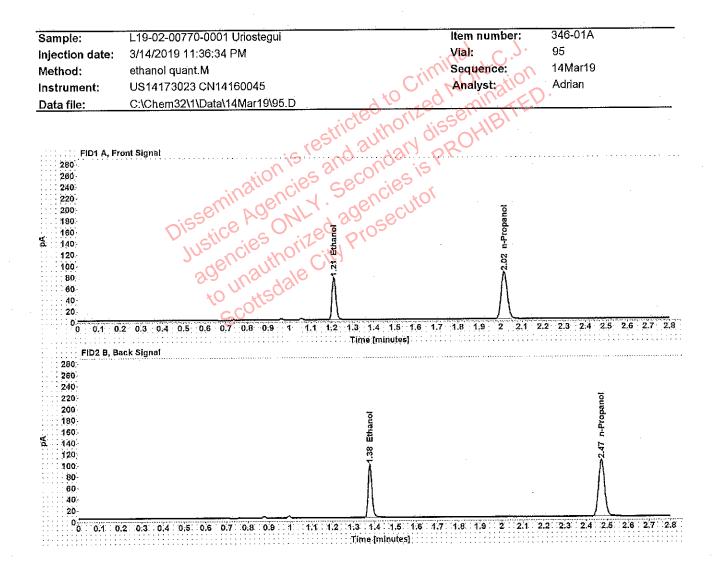


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1520	1.211	96.930
n-Propanol		2.017	168,437

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.377	120.935
n-Propanol	2.473	207.098

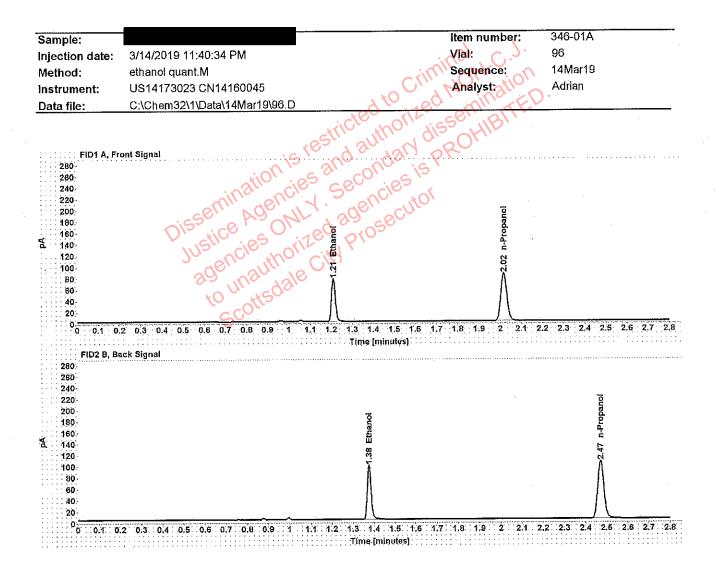


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1513	1.210	97.183
n-Propanol		2.016	169,697

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.376	121.441
n-Propanol	2,472	208,691

User: wadrian 3/18/2019

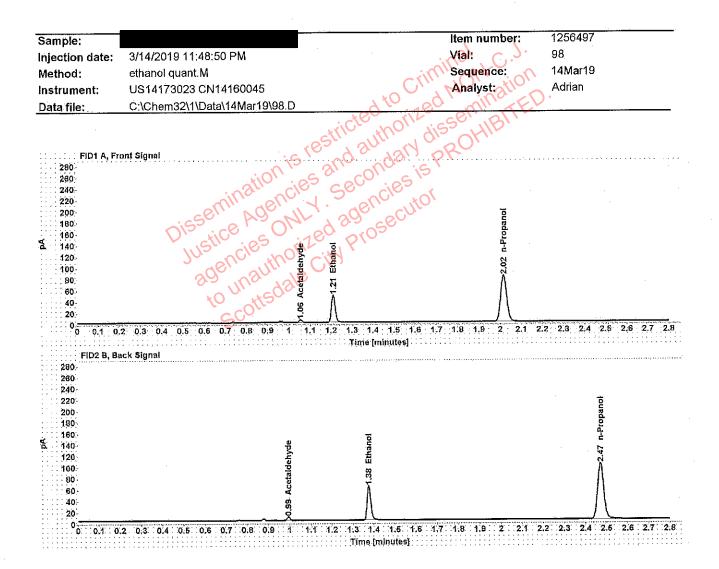


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.908
>Ethanol	0,0996	1.210	62.020
n-Propanol		2.016	165.227

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	6.406
Ethanol	1.376	76,863
n-Propanol	2.471	203.357

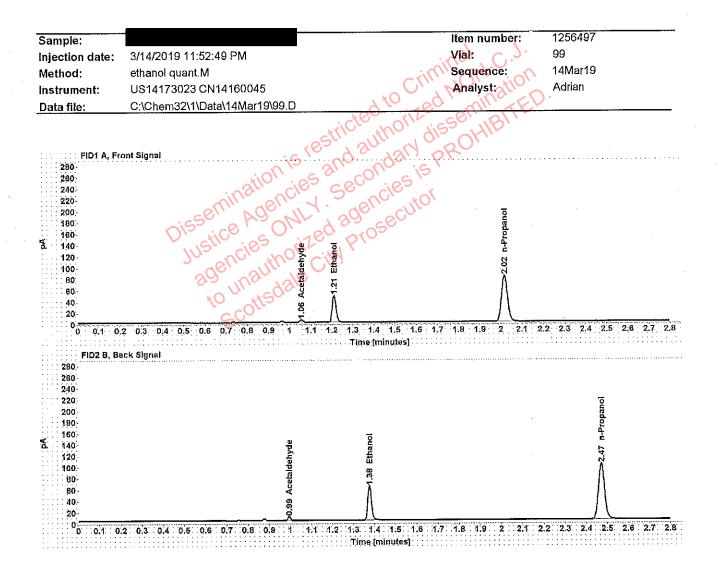


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.997
>Ethanol	0.0997	1.210	61.960
n-Propanol		2.016	164.918

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	6.575
Ethanol	1.376	76.418
n-Propanol	2.471	203.012

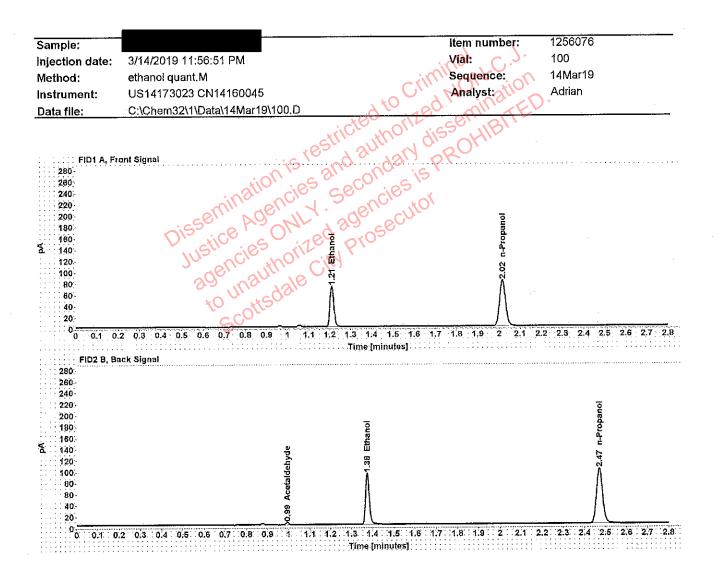


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1499	1,210	92.544
n-Propanol	BARTO	2.016	163.130

Table 2: FID 2 B (column DB-ALC2)

Compound Time (min)		Peak Area
Acetaldehyde	0.994	4.149
Ethanol	1.376	115,328
n-Propanol	2.471	200.874

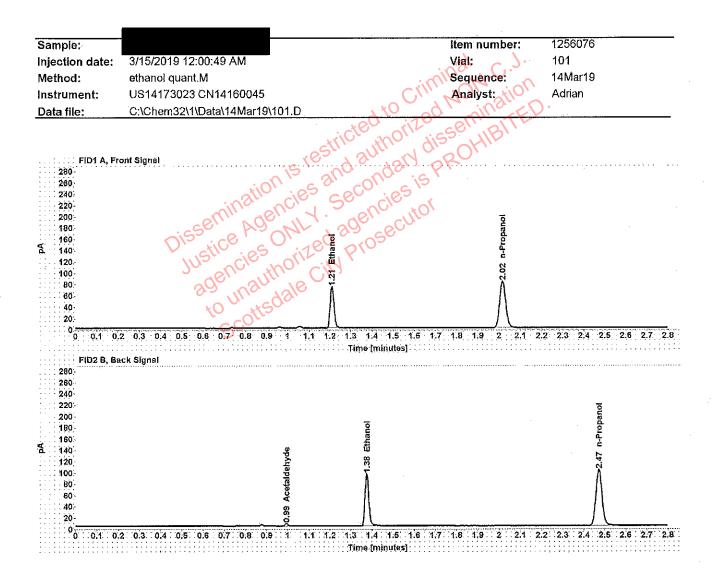


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,1505	1.210	94.017
n-Propanol	AU4300	2,016	165.079

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.131
Ethanol	1.376	116.928
n-Propanol	2.471	203,669