### SCOTTSDALE POLICE DEPARTMENT CRIME LABORATORY BLOOD ALCOHOL FACE SHEET

ANALYSIS DATE	1/15/2019	SEQUENCE NAME	15Jan19	
EQUIPMENT Pipettor Gas Chromatograph	☐ Hamilton ML600EH ⊠ Agilent US1417302		J10749	
INSTRUMENT CAL	IBRATION STILL	authon dissorting		
Vial 1 0.02 calibrator L	ot FN03241604	Coefficient of	determination ( <b>r</b> ²)	
Vial 2 0.10 calibrator L	ot FN06181501 50	0.99999	)	
Vial 3 0.20 calibrator	ot FN07201502	errecuto		
Vial 4 0.40 calibrator	ot FN11191402	(050		
Ju encientho, City				
CALIBRATION VERIFICATION AND RESOLUTION TEST				

Vial	Sample C	Expected result	Measured result	Manufacturer/lot
5	Blank	Not detected	Not detected	SPD lab 121118
6	Volatiles mixture	6 compounds	6 compounds	SPD lab 020917WLA
7	Aqueous control	0.400 g/dL	0.400 g/dL	Lipomed 08012015-C
8	Aqueous control	0.040 g/dL	0.039 g/dL	Lipomed 09022015-A
9	Blood control	0.198 g/dL	0.197 g/dL	ACQ 407041529/13
20	Aqueous control	0.080 g/dL	0.079 g/dL	Lipomed 28082014-B
31	Aqueous control	0.150 g/dL	0.152 g/dL	Lipomed 09022015-C
42	Blood control	0.198 g/dL	0.200 g/dL	ACQ 407041529/13
53	Aqueous control	0.080 g/dL	0.082 g/dL	Lipomed 28082014-B
64	Aqueous control	0.150 g/dL	0.150 g/dL	Lipomed 09022015-C
69	Aqueous control	0.400 g/dL	0.405 g/dL	Lipomed 08012015-C
70	Aqueous control	0.040 g/dL	0.039 g/dL	Lipomed 09022015-A
71	Blood control	0.198 g/dL	0.200 g/dL	ACQ 407041529/13
72	Blank	Not detected	Not detected	SPD lab 121118

### SUBJECT SAMPLES

Subjects	in	the	seque	nce
000000		Q 1 Q	00940	

Subjects requiring reanalysis \_\_\_\_0

ADDITIONAL NOTES: All testing proceeded as expected.

27

20


Run valid Analyst Run valid Mul Biyle / //e/19 Run invalid Analyst Run invalid Technical Reviewer


Document ID: **1208** Revision Date:02/27/2017 Issuing Authority: Kris Cano, Forensic Laboratory Manager Page 1 of 1

# Scottsdale Police Department Crime Laboratory Sequence Quality Assurance Summary

SEQUENCE NAME: 15Jan	19		-	inal C.	ANALYST: Adrian	fu l
Sample Name	Vial	Measured Value (g/dL)	Expected Value (g/dL)	Percent Difference	Absolute Difference (g/dL)	
blank 121118	5	negative	negative	and a	-	
0.400 08012015-C	7	0.400	0,400	5 0.00	0.000	
0.040 09022015-A	8	0.039	0.040	2.50	-0.001	
0.198 407041529/13	9	0.197	0,198	0.51	-0.001	
0.080 28082014-B	20	0.079	0.080	1.25	-0.001	
0.150 09022015-C	31	0.152	0.150	1.33	0.002	
0.198 407041529/13	42	0.200	0,198	1.01	0.002	
0.080 28082014-B	53	0.082	0.080	2.50	0.002	
0.150 09022015-0.5	64	0.150 2 2	0,150	0.00	0.000	
0.40 08012015-0	69	G 0.4050	0100.400	1.25	0.005	
0.04 09022015-A	70	0.039	0.040	2.50	-0.001	
0.198 407041529/13	71	0.200	0.198	1.01	0.002	
blank 121118 🔗 🏸	72	negative	negative	-	-	
<u> </u>	0.	tsoc		,		

Calibrator	Ethanol Area	N-propanol Area	Ratio
0.020	12.888	168.427	0.077
0.100	63.585	165.224	0.385
0.200	129.627	166.625	0.778
0,400	257.981	165.919	1.555

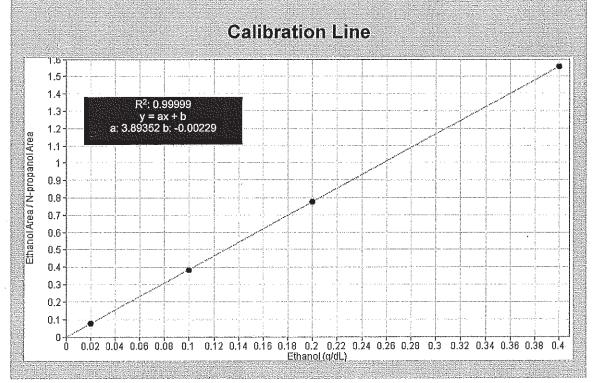


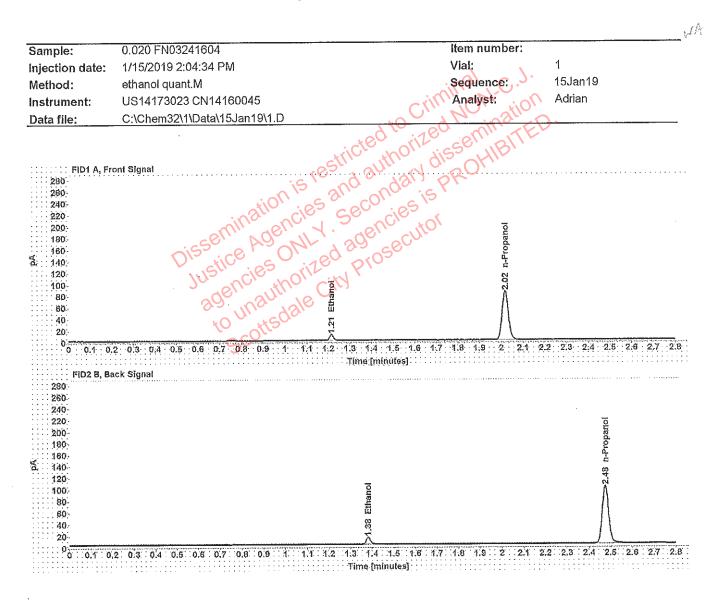

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.214	12.888
n-Propanol	2.017	168.427


Compound	Time (min)	Peak Area
Ethanol	1,381	15.663
n-Propanol	2.475	202.794

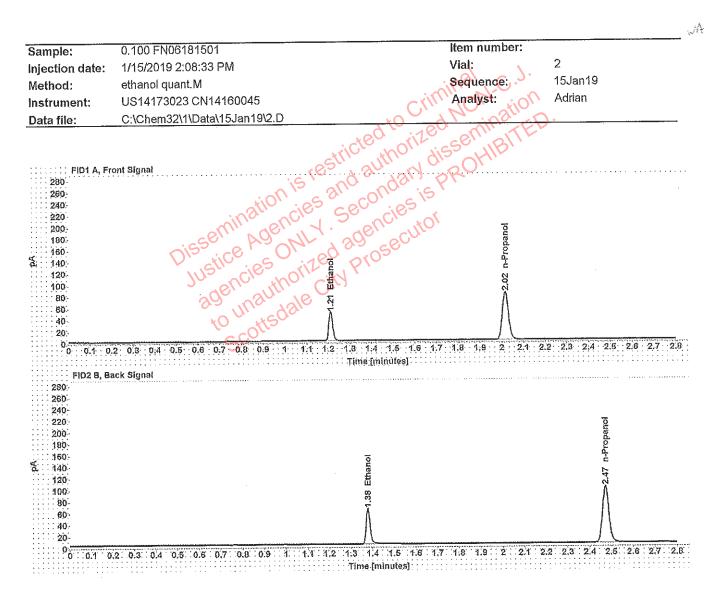

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.210	63.585
n-Propanol	2.016	165.224


Compound	Time (min)	Peak Area
Ethanol	1.378	78.196
n-Propanol	2.473	199,581

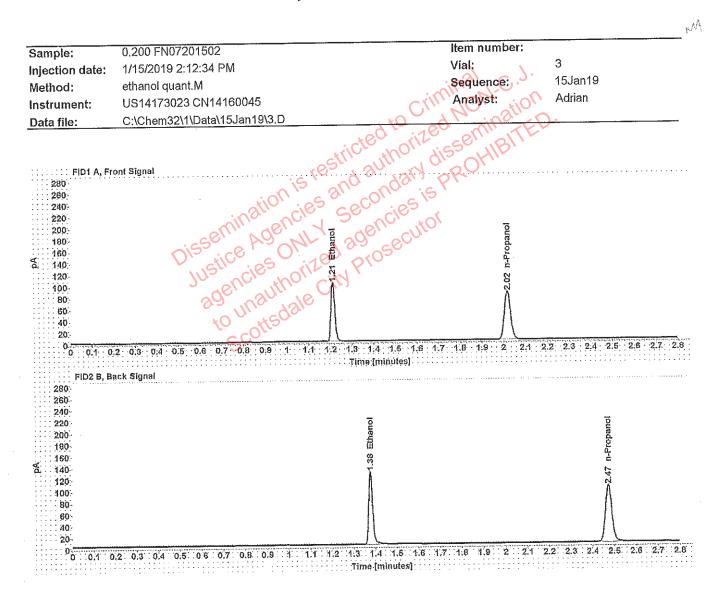

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.210	129.627
n-Propanol	2.016	166.625

Compound	Time (min)	Peak Area
Ethanol	1.377	160.005
n-Propanol	2.473	201,988

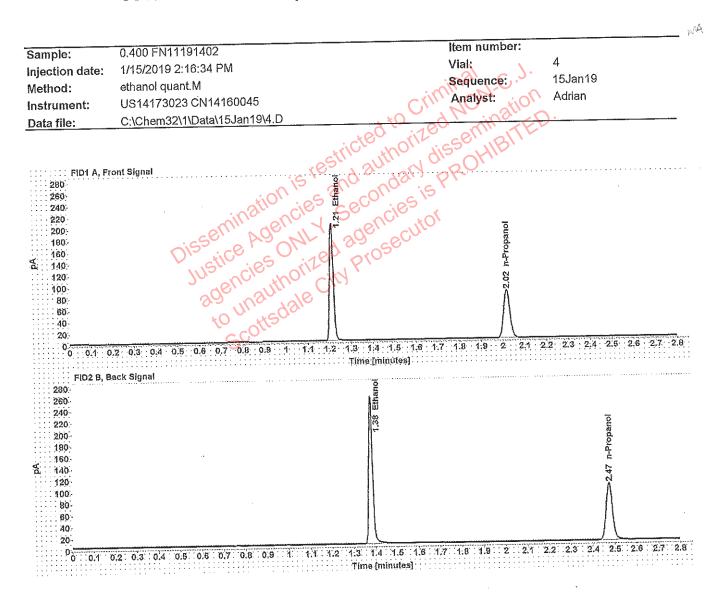

### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.209	257.981
n-Propanol	2.016	165.919

Compound	Time (min)	Peak Area
Ethanol	1.377	319.721
n-Propanol	2.474	201.507

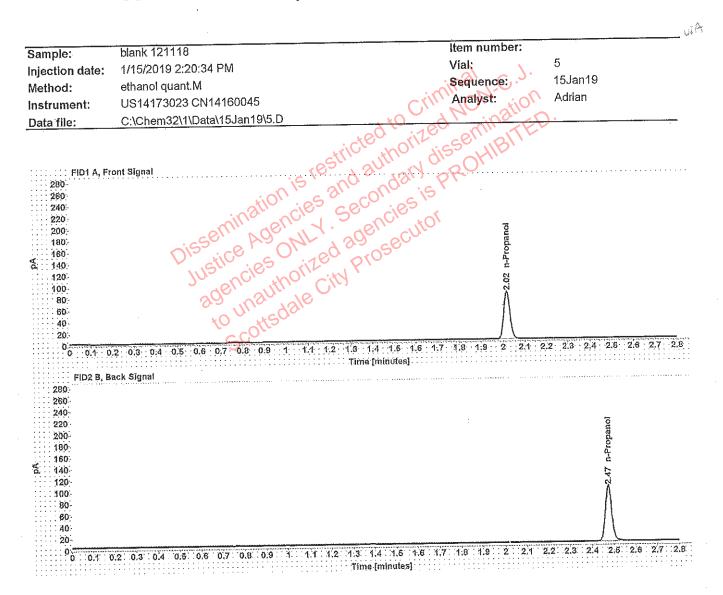


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.017	164.063

Compound	Time (min)	Peak Area
n-Propanol	2.474	198.128

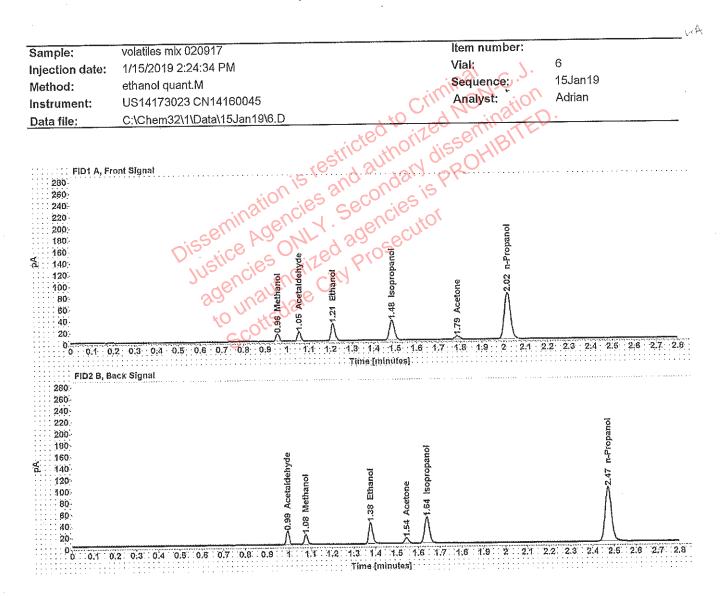


Table 1:	FID 1	A (column	DB-ALC1)
----------	-------	-----------	----------

Compound	Amount (g/100mL)	Time (min)	Peak Area
Methanol		0.957	14.413
Acetaldehyde		1.055	17.490
>Ethanol	0.0617	1.210	38,148
Isoprepanol		1.484	55.067
Acetone		1.786	10.215
n-Propano!		2.016	160.412

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	22.719
Methanol	1.078	18.151
Ethanol	1.377	46,699
Acetone	1.545	12.120
Isopropanol	1,639	69.089
n-Propanol	2.472	194.270

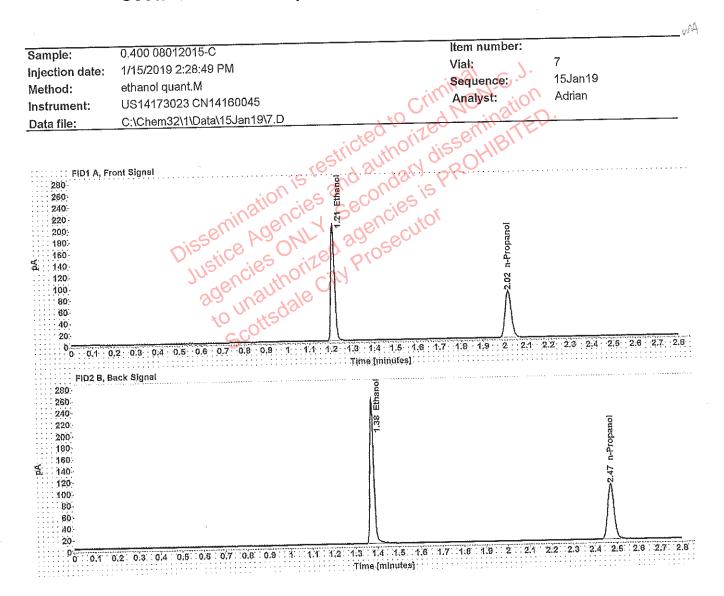


Table 1: FID 1	A (column	DB-ALC1)
----------------	-----------	----------

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.4008	1.208	253.418
n-Propanol		2.016	162.634

Compound	Time (min)	Peak Area
Ethanol	1.376	313,850
n-Propanol	2.472	197.310

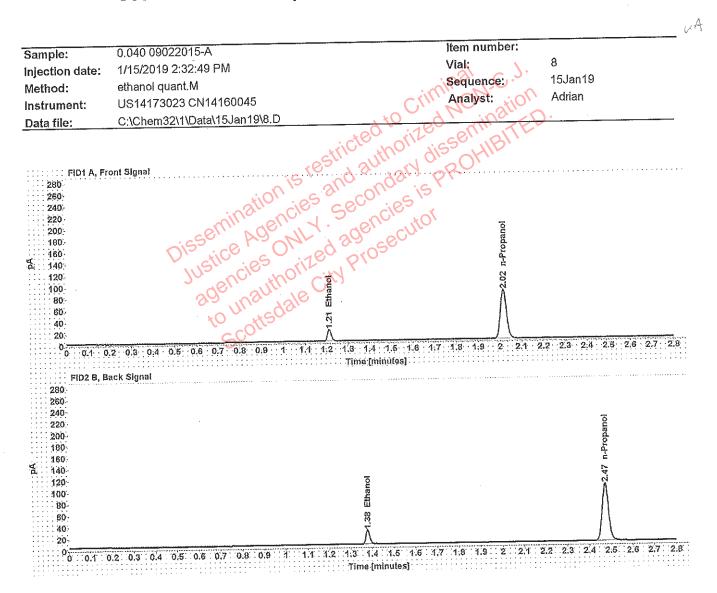


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0396	1.211	25.513
n-Propanol		2.016	167.982

Compound	Time (min)	Peak Area
Ethanol	1.378	31.140
n-Propanol	2.473	203.286

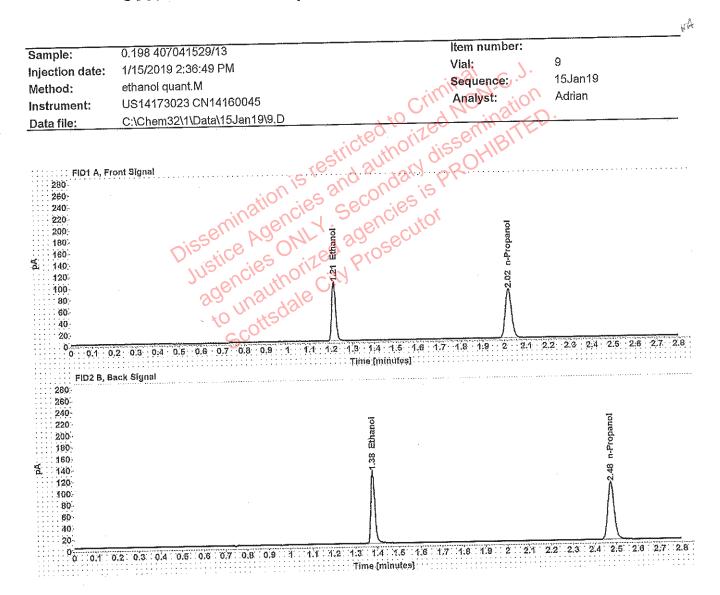


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1975	1.211	129.845
n-Propanol		2.018	169.390

Compound	Time (min)	Peak Area
Ethanol	1.380	160.292
n-Propanol	2.476	205.102

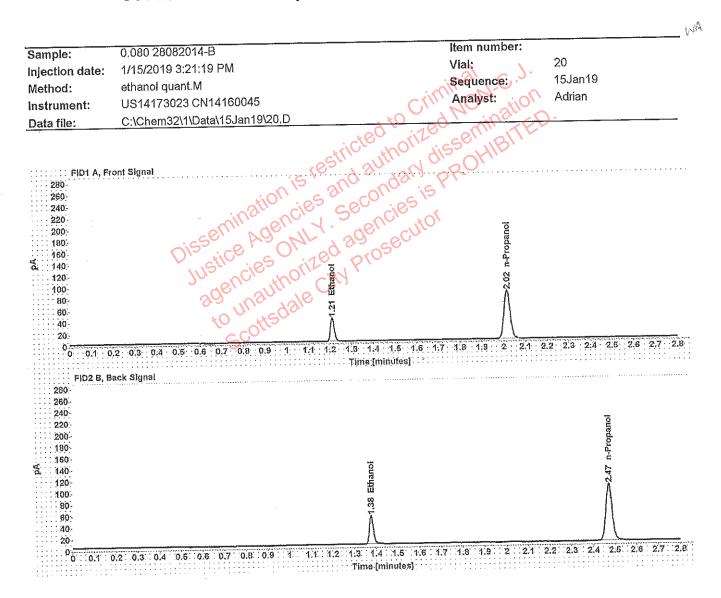


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0795	1.210	51.269
n-Propanol		2.016	166.871

Compound	Time (min)	Peak Area
Ethanol	1.377	62,963
n-Propanol	2.472	202.118

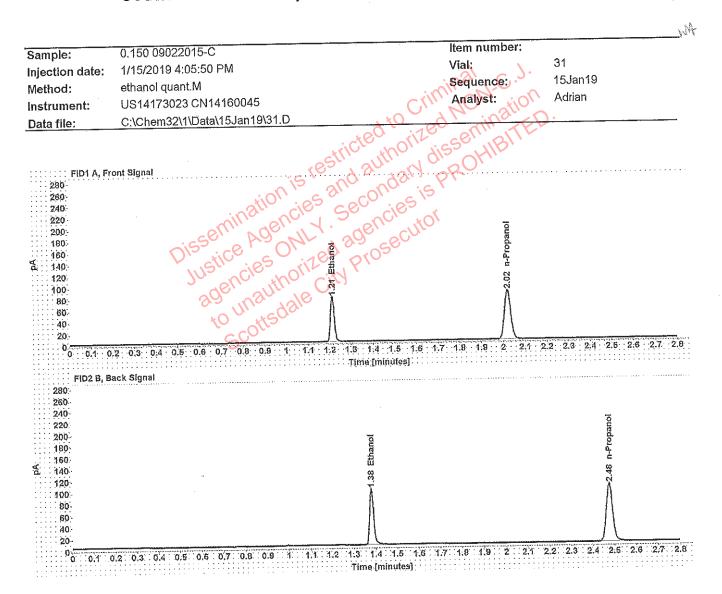


Table 1:	FID 1	A (column	DB-ALC1)
----------	-------	-----------	----------

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1525	1.212	100.575
n-Propanol		2.018	169.992

Compound	Time (min)	Peak Area
Ethanol	1.381	124.023
n-Propanol	2.476	206.291

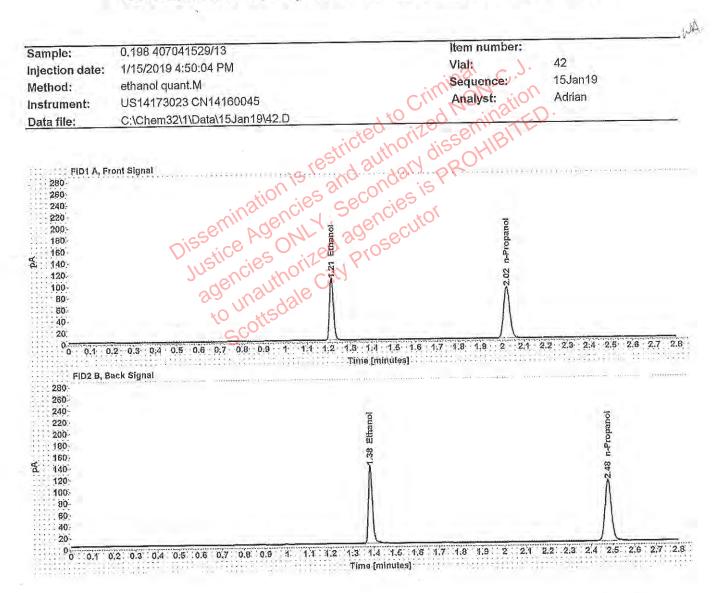


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,2000	1.213	137,870
n-Propanol		2.020	177.608

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.383	170.767
n-Propanol	2.479	216,481

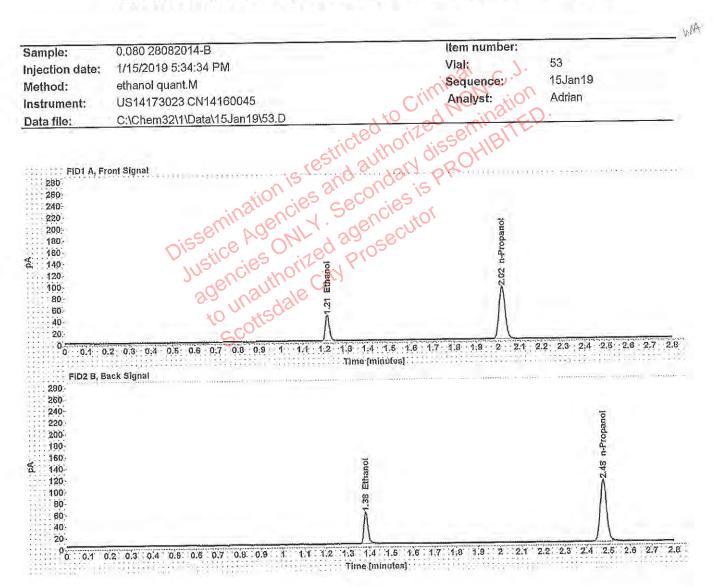


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0821	1.212	57.079
n-Propanol		2.018	179.942

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.381	70.399
n-Propanol	2.476	219.014

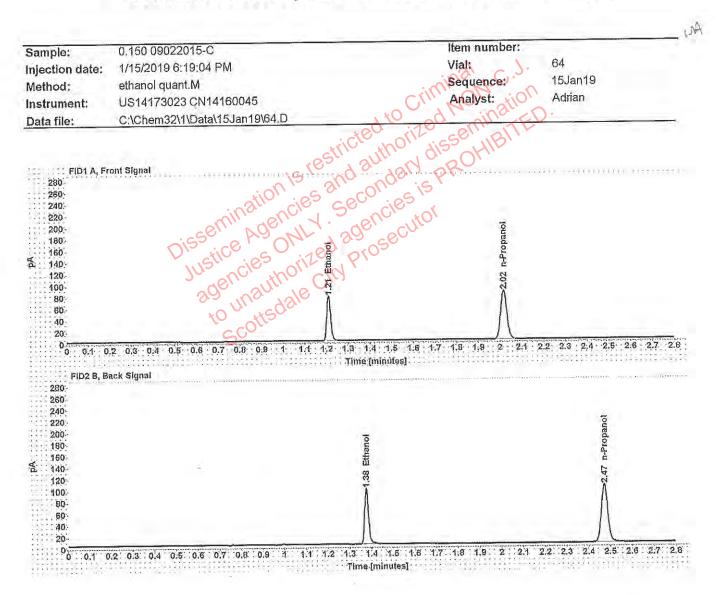


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1500	1.209	98.165
n-Propanol		2.016	168.796

Compound	Time (min)	Peak Area
Ethanol	1.376	121.423
n-Propanol	2.472	205.499

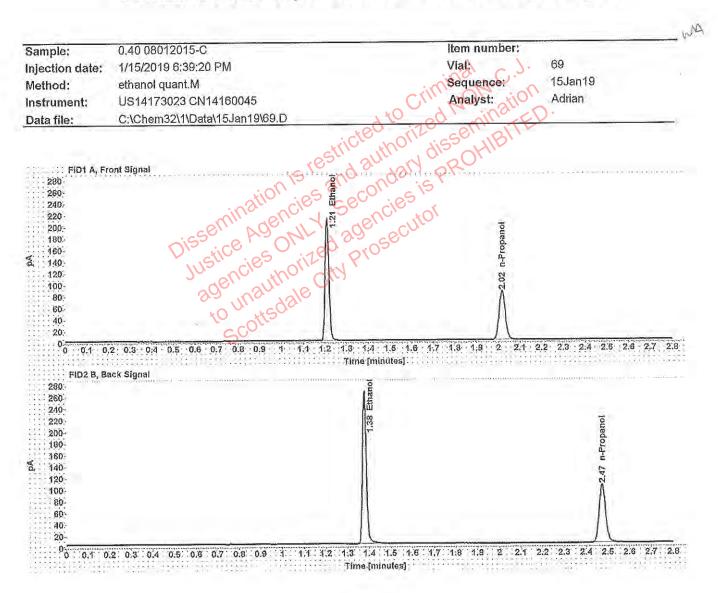


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.4051	1.209	266.523
n-Propanol		2.017	169.215

Compound	Time (min)	Peak Area
Ethanol	1.377	332.556
n-Propanol	2.474	206.778


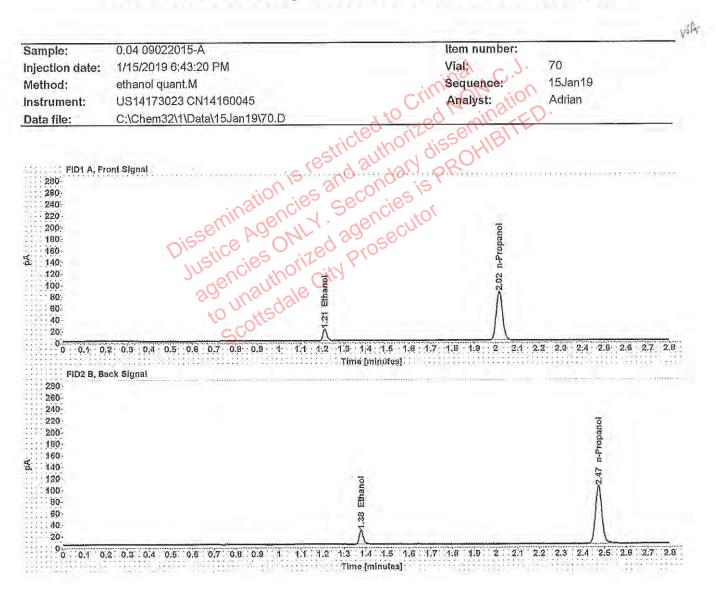


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0393	1.211	25,441
n-Propanol		2.016	168.618


Compound	Time (min)	Peak Area
Ethanol	1.377	31.229
n-Propanol	2.472	205.394

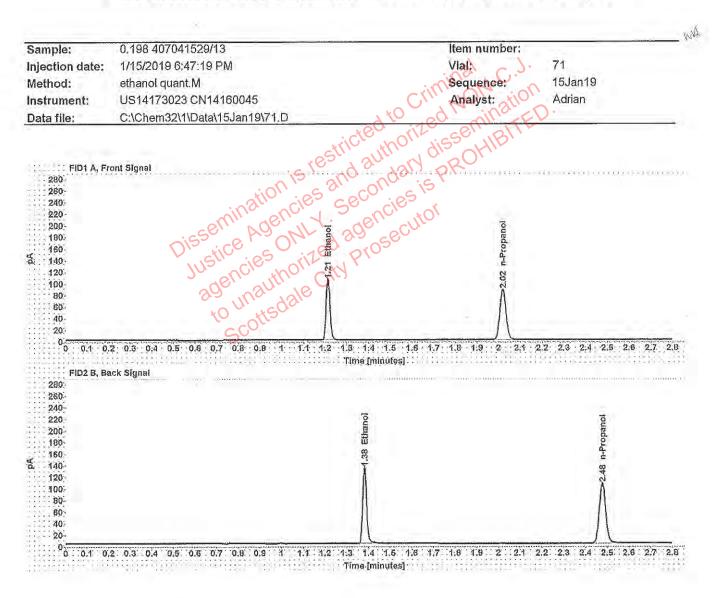

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2007	1.212	136,158
n-Propanol		2.019	174.754

Compound	Time (min)	Peak Area
Ethanol	1.381	168.779
n-Propanol	2,477	213,426

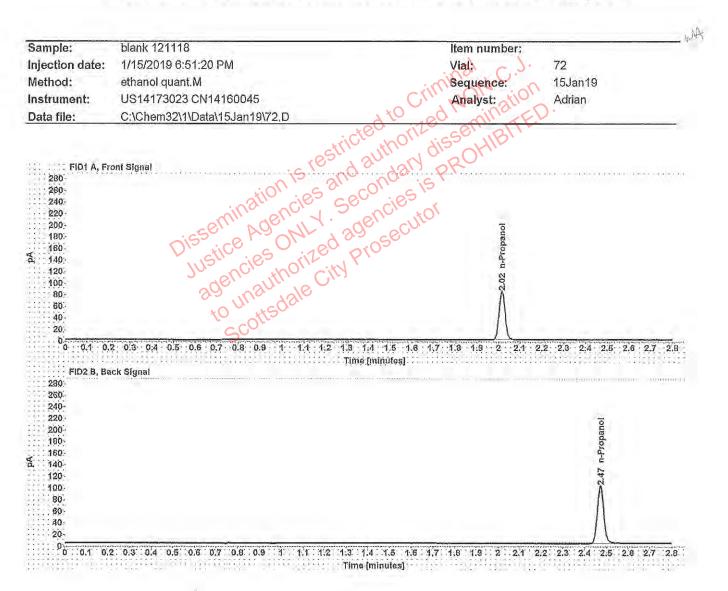

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.015	167.870

Compound	Time (min)	Peak Area
n-Propanol	2.472	204.082

### Sequence Summary

Page 1 of 2

quen	ice name: 15Jan19 Instrument: U	S14173023 CN141	60045 A	nalyst: Adrian
			Ina J.C.C	11 H
Vial	Sample	Туре	Item Number	Method
1	0.020 FN03241604	Calibration		ethanol quant.M
2	0.100 FN06181501	Calibration	SCIPSII	ethanol quant.M
3	0.200 FN07201502	Calibration		ethanol quant.M
4	0.400 FN11191402	Calibration		ethanol quant.M
5	blank 121118	Control	- 10 - 10 - 10 - 10 - 10 - 10 - 10 - 10	ethanol quant.M
6	volatiles mix 020917	Control		ethanol quant.M
7	0.400 08012015-C	Control		ethanol quant.M
8	0.040 09022015-AS	Control		ethanoi quant.M
9	0.198 407041529/13	Control		ethanol quant.M
10	Jue note hollowith	Sample	1219670	ethanol quant.M
11	aller a dilling of the	Sample	1219670	ethanol quant.M
12	and une date	Sample	1078772	ethanol quant.M
13		Sample	1078772	ethanol quant.M
14	So	Sample	1249280	ethanol quant.M
15		Sample	1249280	ethanol quant.M
16		Sample	1249159	ethanol quant.M
17		Sample	1249159	ethanol quant.M
18		Sample	1231554	ethanol quant.M
19		Sampie	1231554	ethanol quant.M
20	0.080 28082014-B	Control		ethanol quant.M
21		Sample	1172130	ethanol quant.M
22		Sample	1172130	ethanol quant.M
23		Sample	1242177	ethanol quant.M
24		Sample	1242177	ethanol quant.M
25		Sample	1251384	ethanol quant.M
26		Sample	1251384	ethanol quant.M
27		Sample	1246474	ethanol quant.M
28		Sample	1246474	ethanol quant.M
29		Sample	1248120	ethanol quant.M
30	an V	Sample	1248120	ethanol quant.M
31	0.150 09022015-C	Control		ethanol quant.M
32		Sample	1249064	ethanol quant.N
33	All wards which all a second	Sample	1249064	ethanol quant.M
33		Sample	1245968	ethanoi quant.M
35		Sample	1245968	ethanol quant.N
36		Sample	1248887	ethanol quant.M
37		Sample	1248887	ethanol quant.M
38		Sample	1247279	ethanol quant.N
39		Sample	1247279	ethanol quant.M
40		Sample	1247996	ethanol quant.M
40		Sample	1247996	ethanol quant.N
	0.198 407041529/13	Control		ethanol quant.N
42	0,130 40/04 (023/13	Sample	1247862	ethanol quant.M
43		Sample	1247862	ethanol quant.N
44		Sample	1248881	ethanol guant.N
45		Sample	1248881	ethanol quant.N
46		Sample	1250798	ethanol quant.M

wA

### Sequence Summary

### 15 J. ~ 14 WA BIS 74

Page 2 of 2

48		Sample	1250798	ethanol quant.M
49		Sample	1251388	ethanol quant.M
50		Sample :	1251388	ethanol quant.M
51		Sample	1251264	ethanol quant.M
52		Sample	1251264	ethanol quant.M
53	0.080 28082014-B	Control	SETB	ethanol quant.M
54	SUT	Sample, O	1251491	ethanol quant.M
55	······································	Sample 🗸	1251491	ethanol quant.M
56	and a state of the	Sample	1244066	ethanol quant.M
57		Sample	1244066	ethanol quant.M
58		Sample	1248899	ethanol quant.M
59	icse Pool 20	Sample	1248899	ethanol quant.M
60	D <sup>I</sup> tice a ile i	Sample	1250243	ethanol quant.M
61	this one way	Sample	1250243	ethanol quant.M
62		Sample	1250324	ethanol quant.M
63		Sample	1250324	ethanol quant.M
64	0,150 09022015-C	Control		ethanol quant.M
65		Sample	1249183	ethanol quant.M
66		Sample	1249183	ethanol quant.M
67	an Su Santa	Sample	1248868	ethanol quant.M
68		Sample	1248868	ethanol quant.M
69	0.40 08012015-C	Control		ethanol guant.M
70	0.04 09022015-A	Control		ethanol quant.M
71	0.198 407041529/13	Control		ethanol quant.M
72	blank 121118	Control		ethanol guant.M

# Scottsdale Police Department Crime Laboratory Summary of Cases

SECHEN	SEQUENCE NAME: 15Jan19 ANALYST: Adrian				
Vials	Test 1 (g/dL)	Test 2 (g/dL)	Mean (g/dL)	Percent Difference*	Absolute Difference (g/dL)*
10 11	0.1872	0.1836	0.18540	0.97	0.00180
12 13	0,1540	0.1563	0.15515	0.74	0.00115
14 15	0.0000	0.0000	0.00000	0.00	0.00000
16 17	0.1590	0.1625	0.16075	1.09	0.00175
18 19	0.1010	0,1014 💉	0,10120	0.20	0.00020
21 22	0,1505	0.1494	0.14995	0.37	0.00055
23 24	0.1924	0.1962	0,19430' 📿	0.98	0.00190
25 26	0.0000	00000 0	0.00000 5	0.00	0.00000
27 28	0.3147	0.3206	0.31765	0.93	0.00295
29 30	0.1775	0,1769	0.17720	0,17	0.00030
32 33	0.1572	0.1563	0.15675	0.29	0.00045
34 35	0.1068	0.1064	0,10660	0.19	0.00020
36 37	0,1975,600	. 05 0.1949	0.19620	0.66	0.00130
38 39	0.1489	0.1474	0.14815	0.51	0.00075
40 41	0.2197	0.2210	0.22035	0.29	0.00065
43 44	0.0838	0.0822	0.08300	0.96	0.00080
45 46	0.2358 10	0.2337	0.23475	0.45	0.00105
47 48	0.1223	0.1215	0.12190	0.33	0.00040
49 50	0.0598	0.0599	0.05985	0.08	0.00005
51 52	0.0722	0.0722	0.07220	0.00	0.00000
54 55	0.0776	0.0772	0.07740	0.26	0.00020
56 57	0.1327	0,1322	0.13245	0.19	0.00025
58 59	0.2121	0.2096	0.21085	0.59	0.00125
60 61	0.1379	0.1369	0.13740	0.36	0.00050
62 63	0.0949	0.0973	0.09610	1.25	0.00120
65 66	0.1652	0.1657	0.16545	0.15	0.00025
67 68	0.1994	0.2008	0.20010	0.35	0.00070


\*Calculated differences are differences from the mean of the two results.

### : Adrian, William - (16-Jan-2019)

ser: wadrian 1/16/2019

#### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

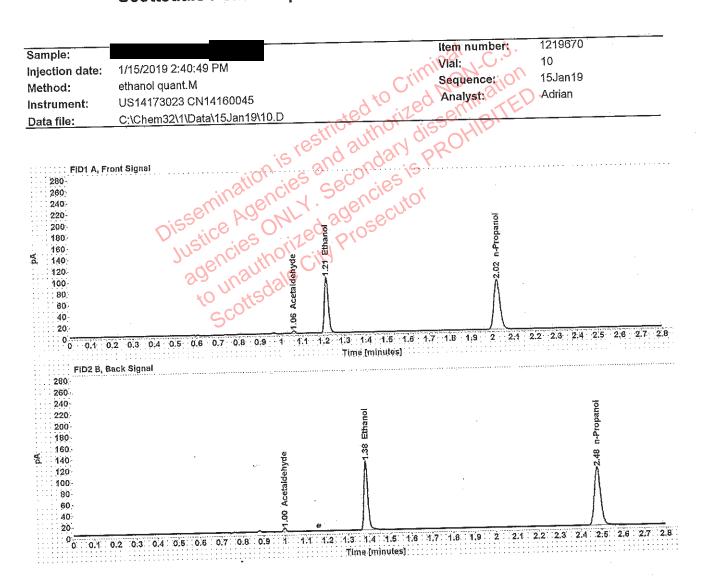


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	4.688
>Ethanol	0.1872	1.214	128.284
n-Propanol		2.020	176.558

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	6.109
Ethanol	1.384	158.419
n-Propanol	2.479	214.189

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

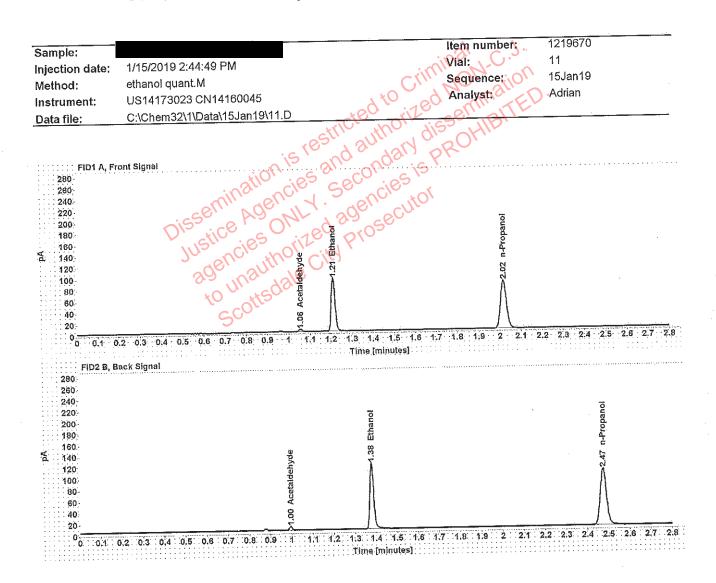

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1,056	4,609
>Ethanol	0.1836	1,211	121.046
n-Propanol		2.017	169.832

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.995	6.022
Ethanol	1.379	148.774
n-Propanol	2.475	205.977

Case:

# Adrian, William - (16-Jan-2019)

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

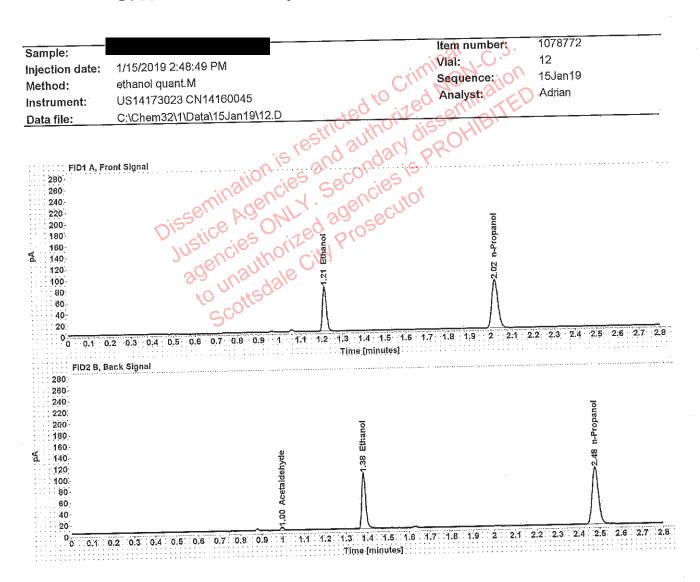


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1540	1,214	103.005
n-Propanol		2.020	172.454

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	4.961
Ethanol	1,383	128.101
n-Propanol	2.479	208.705

Case:

# Adrian, William - (16-Jan-2019)

User: wadrian 1/16/2019



# Scottsdale Police Department Crime Lab Volatiles Analysis

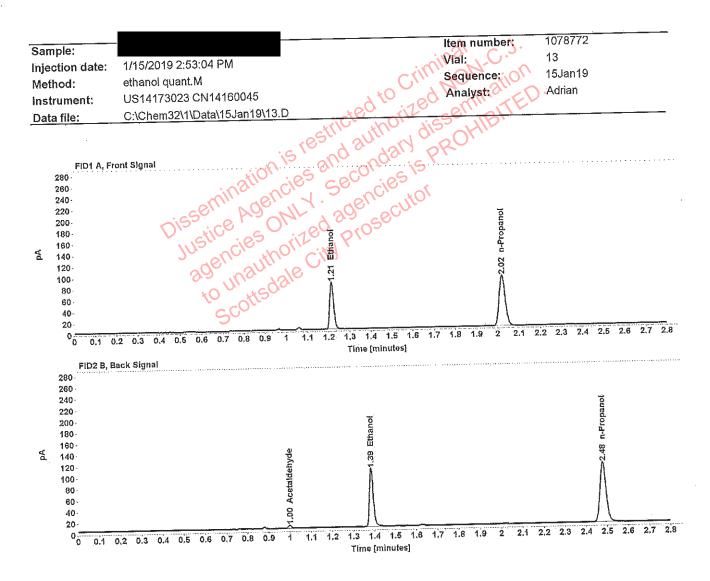


Table	1: FI	) 1 A	(column	DB-ALC	1)	ļ
-------	-------	-------	---------	--------	----	---

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1563	1.215	109.057
n-Propanol		2.021	179.829

Compound	Time (min)	Peak Area
Acetaldehyde	0,999	4.928
Ethanol	1.386	135.326
n-Propanol	2,481	217.651

### <u> Adrian, William - (16-Jan-2019)</u> User: wadrian 1/16/2019

Case:

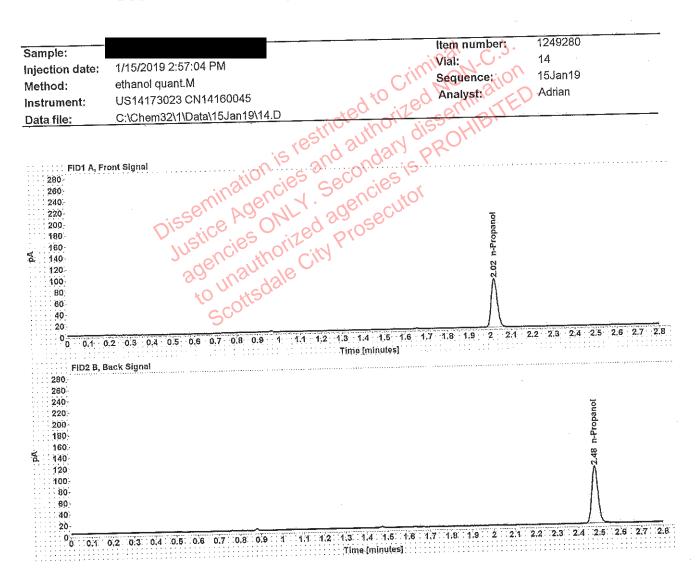


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.020	171.923

Compound	Time (min)	Peak Area
n-Propanol	2.479	208.600

# : Adrian, William - (16-Jan-2019)

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

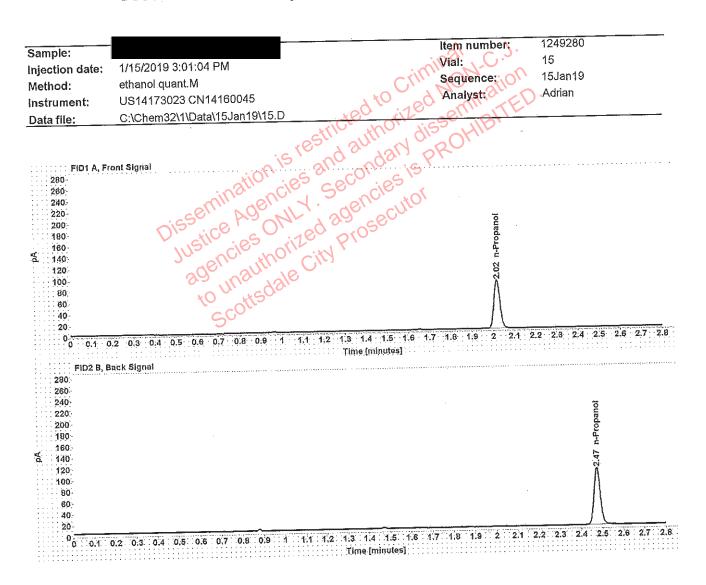

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.017	171.828

### Table 2: FID 2 B (column DB-ALC2)


Compound	Time (min)	Peak Area
n-Propanoi	2.475	208.570

Case:

### : Adrian, William - (16-Jan-2019)

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

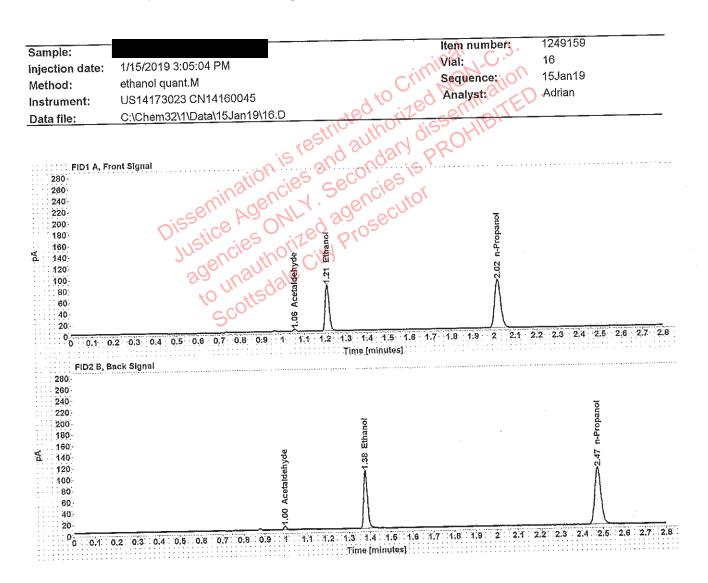

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.056	4.320
>Ethanol	0.1590	1,211	106.290
n-Propanol		2.017	172.277

### Table 2: FID 2 B (column DB-ALC2)


Compound	Time (min)	Peak Area
Acetaldehyde	0.996	5,668
Ethanol	1.379	130.607
n-Propanol	2.475	208.544

Case:

### : Adrian, William - (16-Jan-2019) User: wadrian 1/16/2019

### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

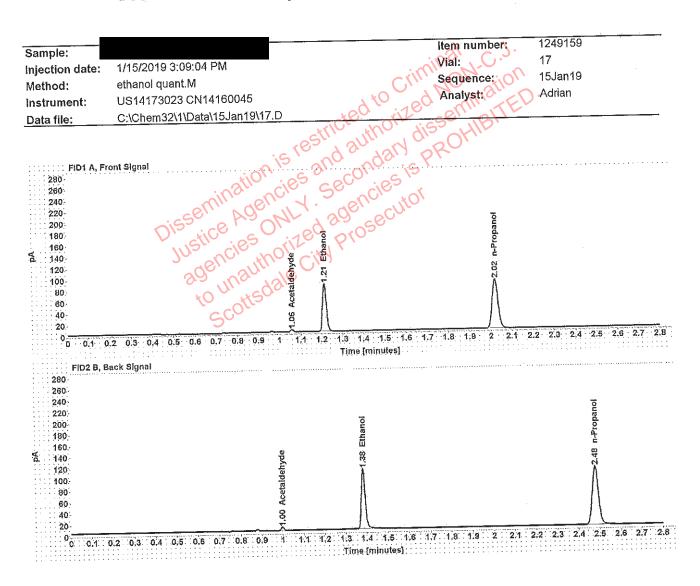

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	4.282
>Ethanol	0.1625	1.214	110.120
n-Propanol		2.020	174.661

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	5.583
Ethanol	1.383	136.551
n-Propanol	2.479	212.071

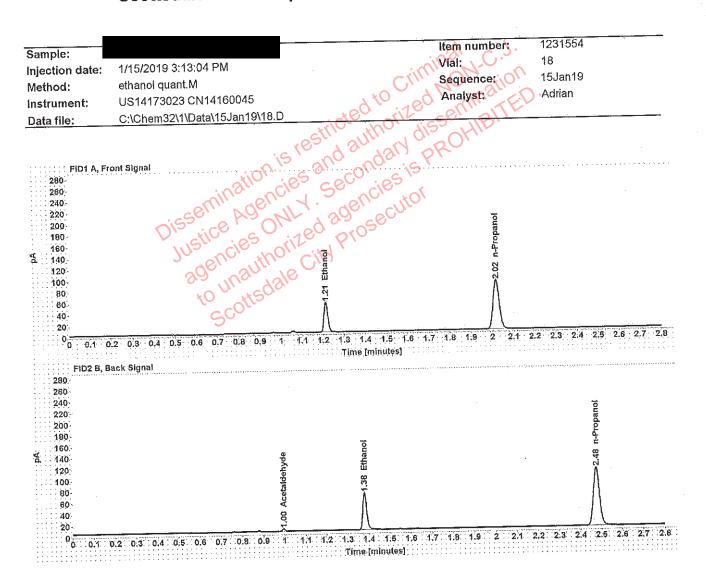


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1010	1.212	68.370
n-Propanol		2.018	174.946

### Table 2: FID 2 B (column DB-ALC2)


Compound	Time (min)	Peak Area
Acetaldehyde	0.996	4.154
Ethanol	1.380	83.875
n-Propanol	2.475	212.451

Case:

### Adrian, William - (16-Jan-2019) User: wadrian 1/16/2019

#### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

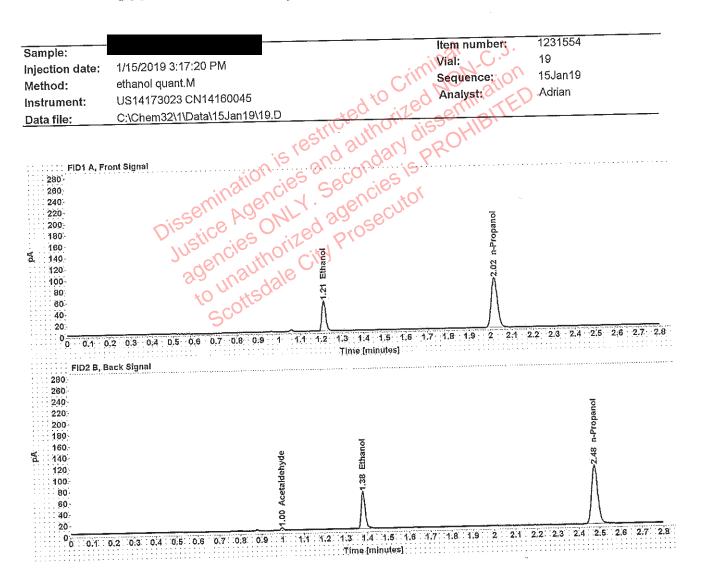

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1014	1.212	69.151
n-Propanol		2.018	176,190


Compound	Time (min)	Peak Area
Acetaldehyde	0.996	4.155
Ethanol	1,381	84.605
n-Propanol	2.476	214.103

### Adrian, William - (16-Jan-2019)

Case:

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

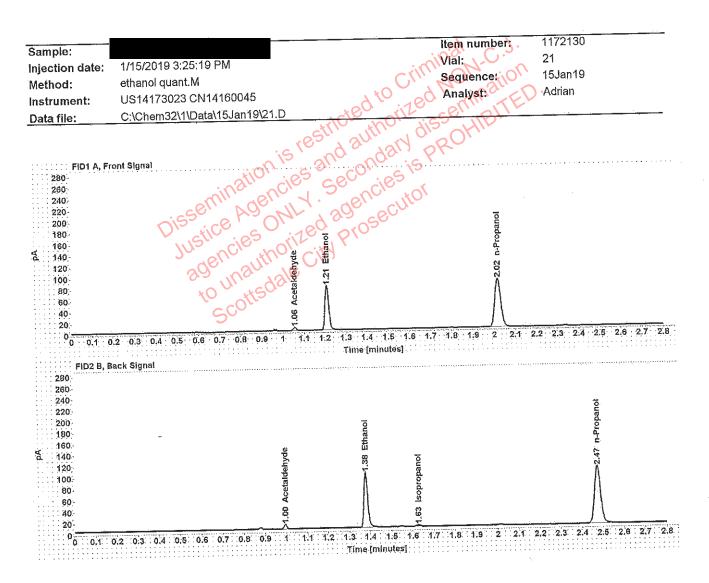


### Table 1: FID 1 Å (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaidehyde		1.056	5.741
>Ethanol	0.1505	1.210	100.452
n-Propanol	*	2.017	172.074

Compound	Time (min)	Peak Area
Acetaldehyde	0.995	7,495
Ethanol	1.378	125.536
Isopropanol	1,626	4.369
n-Propanol	2.474	208.678

Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

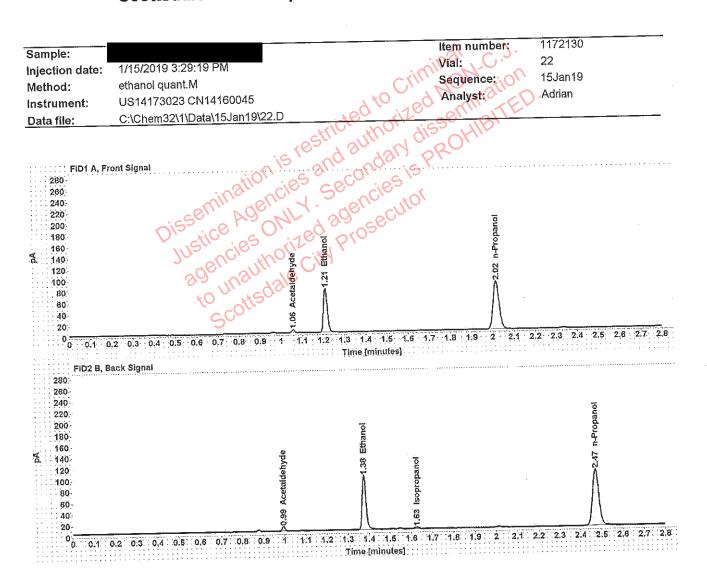

### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	5.814
>Ethanoi	0.1494	1,209	99.270
n-Propanol		2.016	171.384

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	7.631
Ethanol	1.376	123.639
Isopropanol	1.626	4.567
n-Propanol	2.472	206.981

### : Adrian, William - (16-Jan-2019)

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

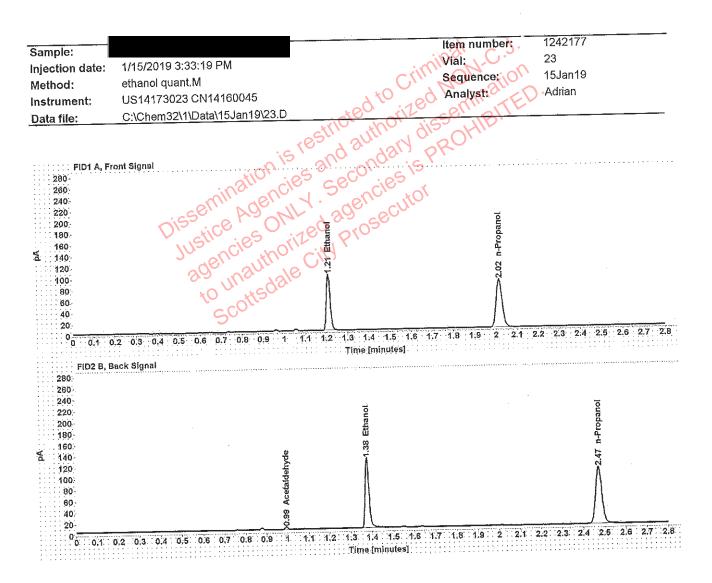

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1924	1,209	126.671
n-Propanol		2,016	169.639


#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.253
Ethanol	1.376	159.088
n-Propanol	2.472	206.577

Case:

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

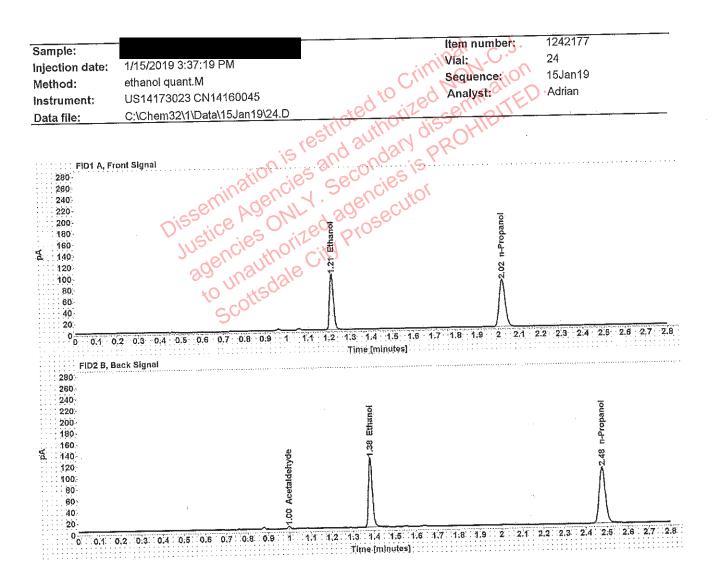

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1962	1,213	127.421
n-Propanol		2.019	167.319

Compound	Time (min)	Peak Area
Acetaldehyde	0.997	4.229
Ethanol	1.382	158.745
n-Propanol	2,478	203.909

Case:

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

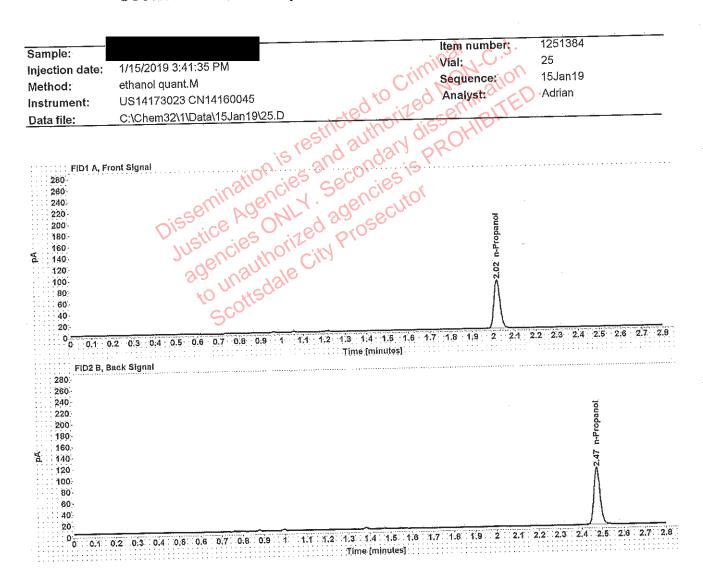



Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2,016	171.953

Compound	Time (min)	Peak Area
n-Propanol	2.473	208.140

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

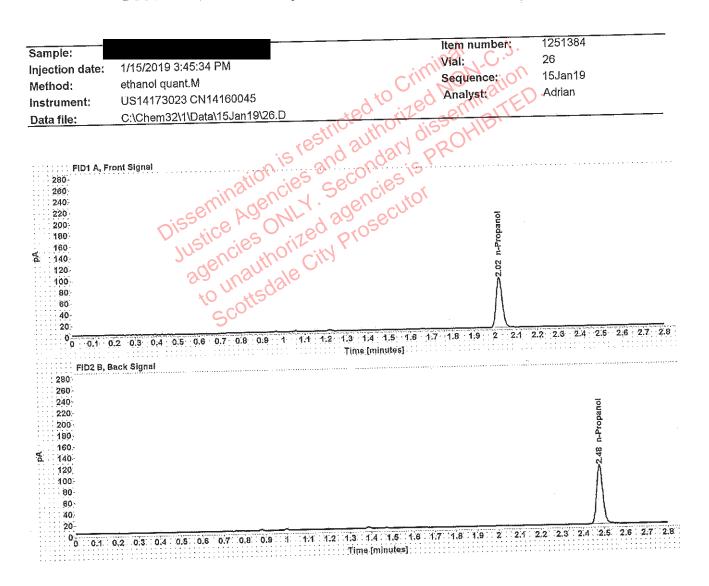

### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
ń-Propanol		2.020	177.069

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2,479	214.701

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

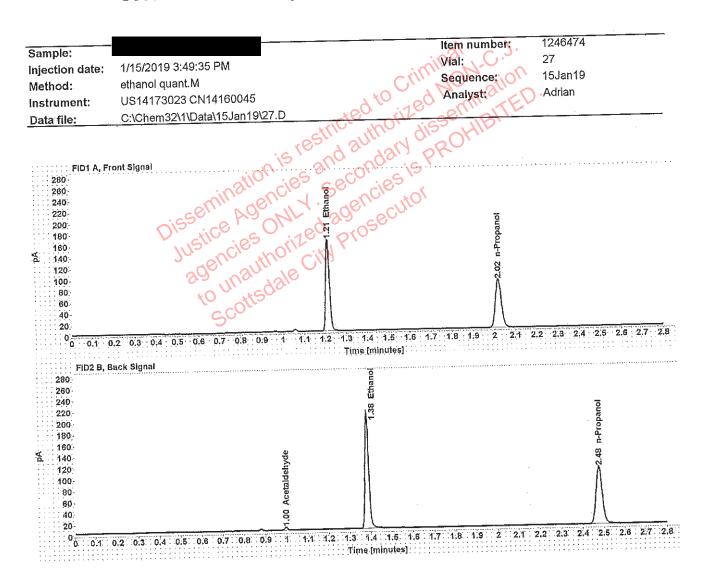

### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.3147	1.212	210,016
n-Propanol		2.019	171.719

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaidehyde	0.997	4,720
Ethanol	1.382	259.487
n-Propanol	2.478	208.983

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

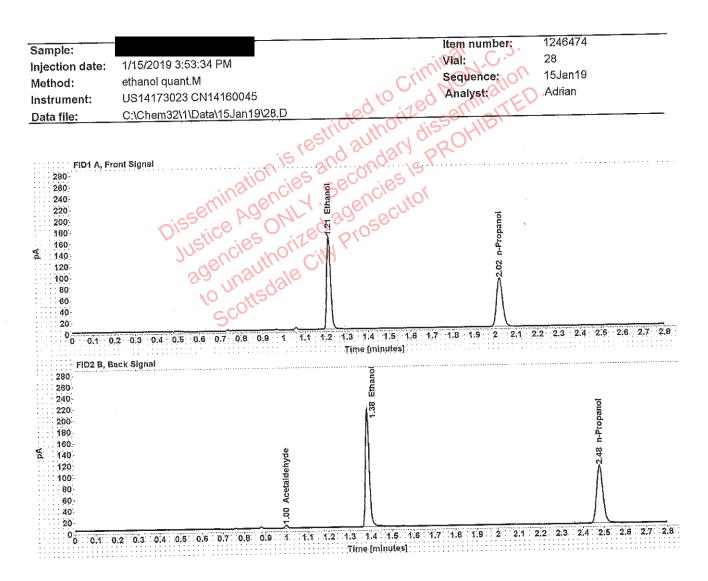

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.3206	1.214	215.145
n-Propanol		2.021	172.667

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldenyde	0.998	4.742
Ethanol	1.384	265.807
n-Propanol	2.480	209.859

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

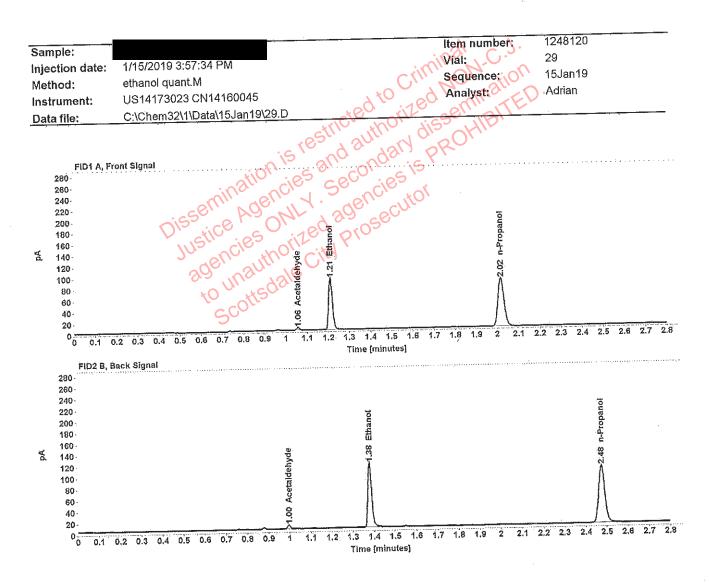


Table 1	FID 1	A (column	DB-ALC1)
---------	-------	-----------	----------


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.056	5.023
>Ethanol	0.1775	1.211	117.781
n-Propanol		2.018	170.975

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.996	6.564
Ethanol	1.380	147.068
n-Propanol	2.476	207.574

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

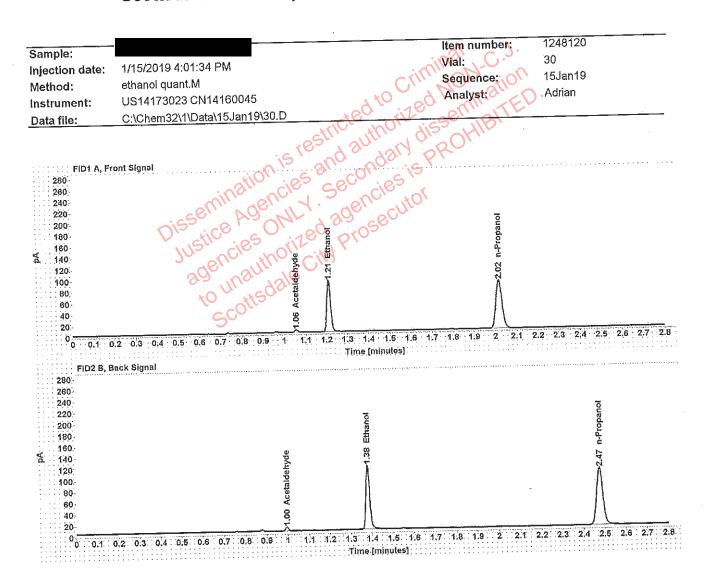


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.056	5.032
>Ethanol	0.1769	1.211	117.837
n-Propanol		2.017	171.680

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.995	6.557
Ethanol	1.379	146.655
n-Propanol	2.475	208.062

# Scottsdale Police Department Crime Lab Volatiles Analysis

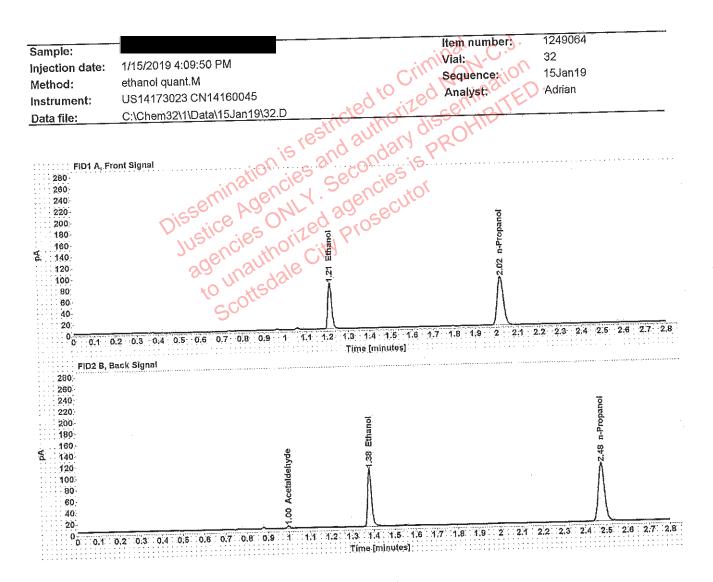

### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,1572	1.212	105,879
n-Propanol		2.019	173.631

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.997	3.765
Ethanol	1.381	132.107
n-Propanol	2.477	210.992

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

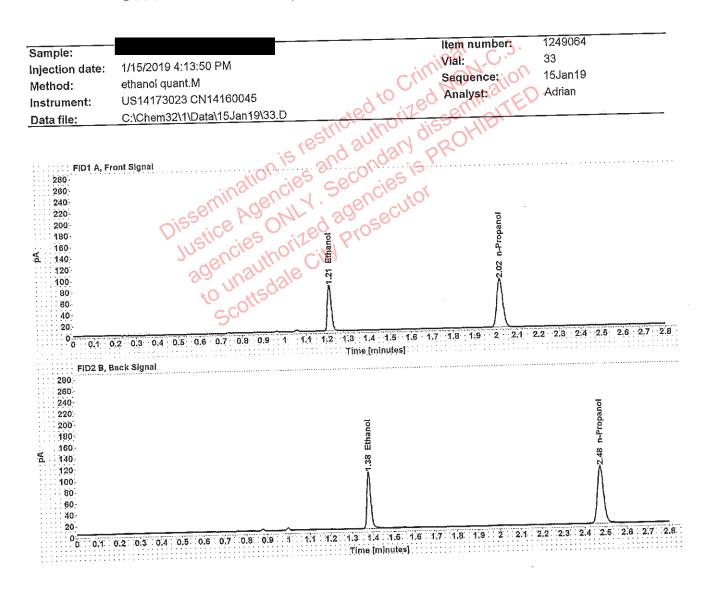


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1563	1.212	104.122
n-Propanol		2.018	171.714

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.381	129,772
n-Propanol	2.477	208.703

# Scottsdale Police Department Crime Lab Volatiles Analysis

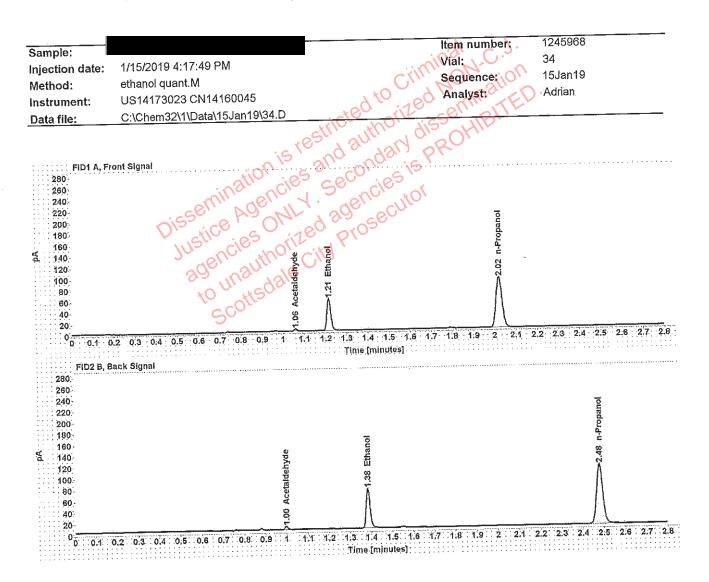

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	4.073
>Ethanol	0.1068	1.214	74.158
n-Propanol		2.020	179,405

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	5,364
Ethanol	1.384	90.560
n-Propanol	2.479	217.881

#### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

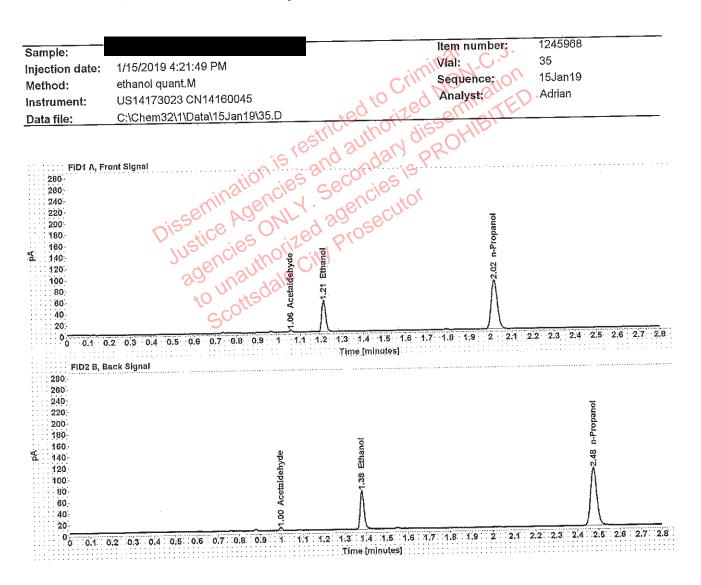


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.056	3.967
>Ethanol	0.1064	1.212	71.530
n-Propanol		2.018	173.611

Compound	Time (min)	Peak Area
Acetaldehyde	0.996	5,168
Ethanol	1.381	87.265
n-Propanol	2.476	210.864

User: wadrian 1/16/2019

### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

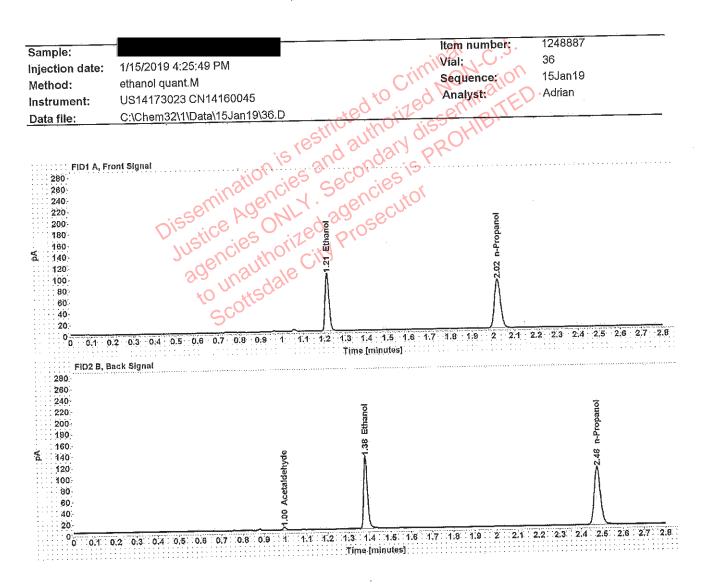


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1975	1.213	132.368
n-Propanol		2.019	172.690

Compound	Time (min)	Peak Area
Acetaldehyde	0.997	4.794
Ethanol	1,382	163.457
n-Propanol	2.478	210.390

# Scottsdale Police Department Crime Lab Volatiles Analysis

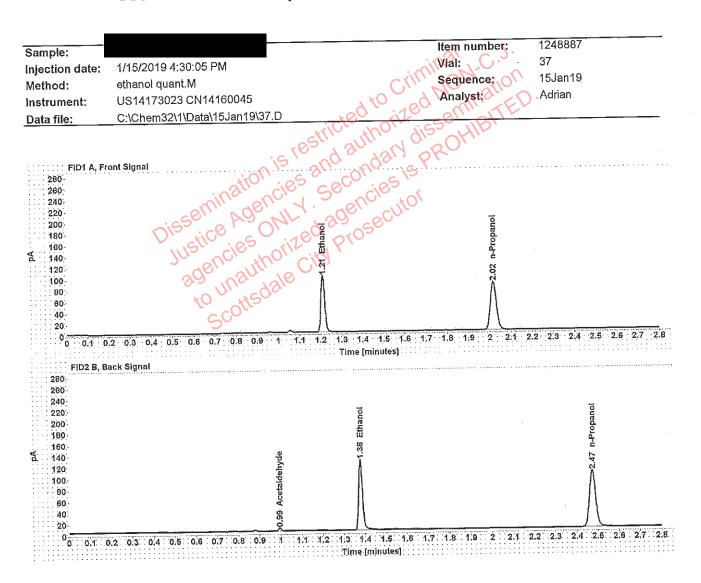

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1949	1.210	128.492
n-Propanol		2.017	169.821


#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.995	4.812
Ethanol	1.378	158.363
n-Propanol	2.474	206,402

Case:

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

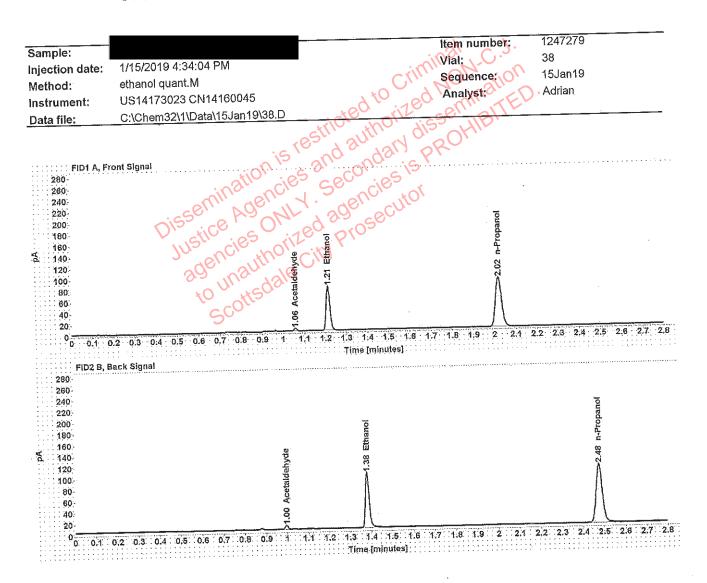


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.056	5.011
>Ethanol	0.1489	1.212	101.193
n-Propanol		2.018	175.249

Compound	Time (min)	Peak Area	
Acetaldehyde	0.996	6.531	
Ethanol	1,380	124.249	
n-Propanol	2.476	213.448	

### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

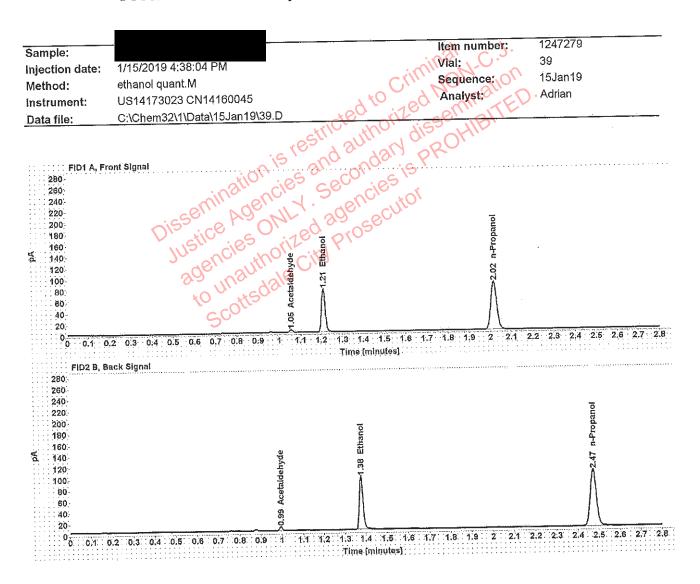

### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4,958
>Ethanol	0.1474	1,209	97.490
n-Propanol		2.016	170.542

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	6,515
Ethanol	1,377	119.726
n-Propanol	2.472	207.302

Case:

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

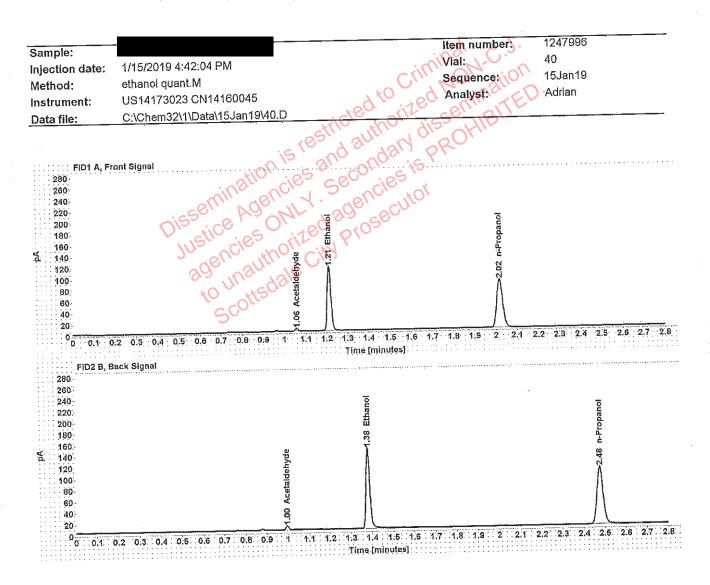


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.056	4.934
>Ethanol	0,2197	1.212	146.623
n-Propanol		2.018	171.883

Compound	Time (min)	Peak Area
Acetaldehyde	0,996	6.502
Ethanol	1,380	181.067
n-Propanol	2.476	208.915

### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

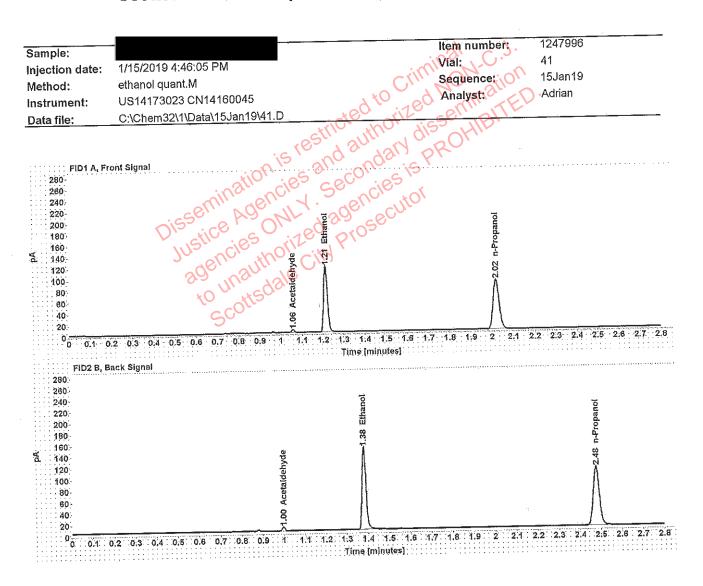


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1,057	4,974
>Ethanol	0.2210	1.212	150.660
n-Propanol		2.018	175.568

Compound	Time (min)	Peak Area
Acetaldehyde	0.997	6.482
Ethanol	1.381	186.322
n-Propanol	2.477	213,980

Case:

Scottsdale Police Department Crime Lab Volatiles Analysis

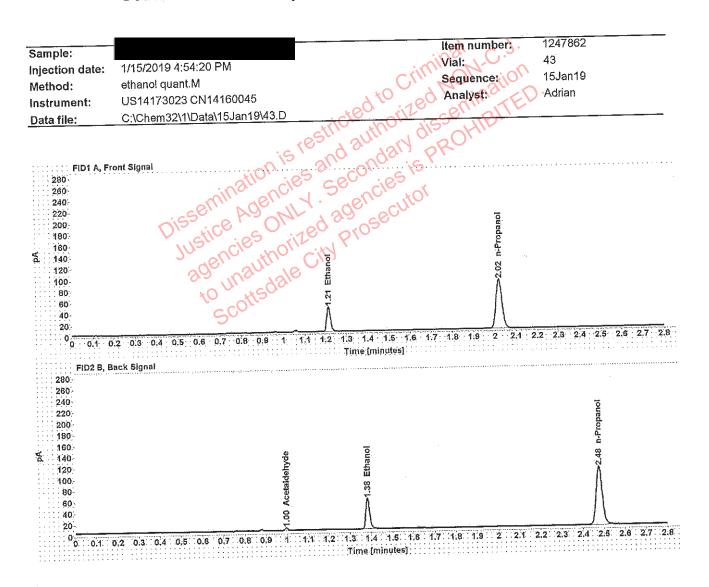


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0838	1.213	56.618
n-Propanol		2,019	174.855

Compound	Time (min)	Peak Area
Acetaldehyde	0,997	4.139
Ethanol	1.383	68.896
n-Propanol	2.478	212.767

# Scottsdale Police Department Crime Lab Volatiles Analysis

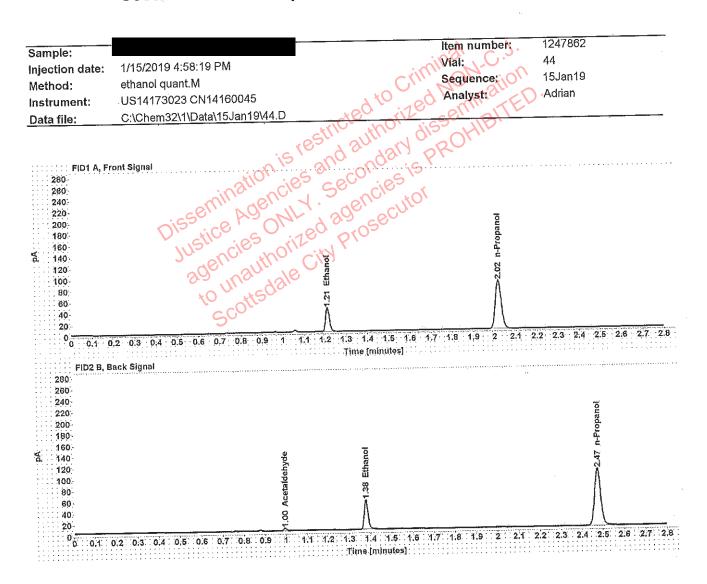

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethano!	0.0822	1.211	54.543
n-Propanol		2.017	171.698

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.995	4.157
Ethanol	1.379	66.784
n-Propanol	2.474	208.931

Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis


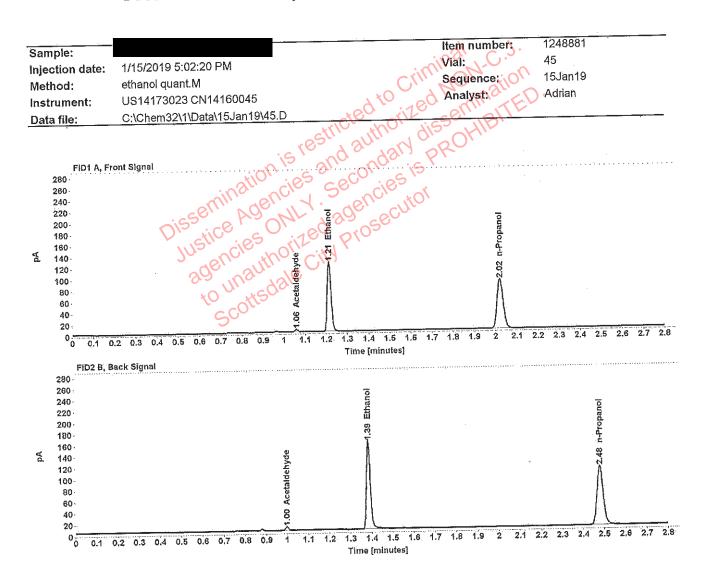


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	4,532
>Ethanol	0,2358	1.214	161.427
n-Propanol		2.021	176.279

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	5.989
Ethanol	1.385	199.268
n-Propanol	2.480	214.944

# Scottsdale Police Department Crime Lab Volatiles Analysis

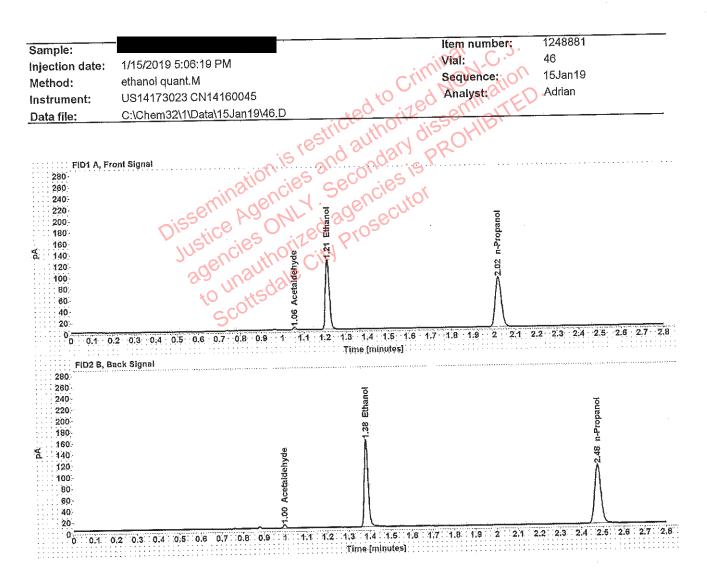

#### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.057	4.580
>Ethanol	0.2337	1.213	160.444
n-Propanol		2.019	176.744

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.997	6.037
Ethanol	1.382	198.248
n-Propanol	2.478	215.656

#### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

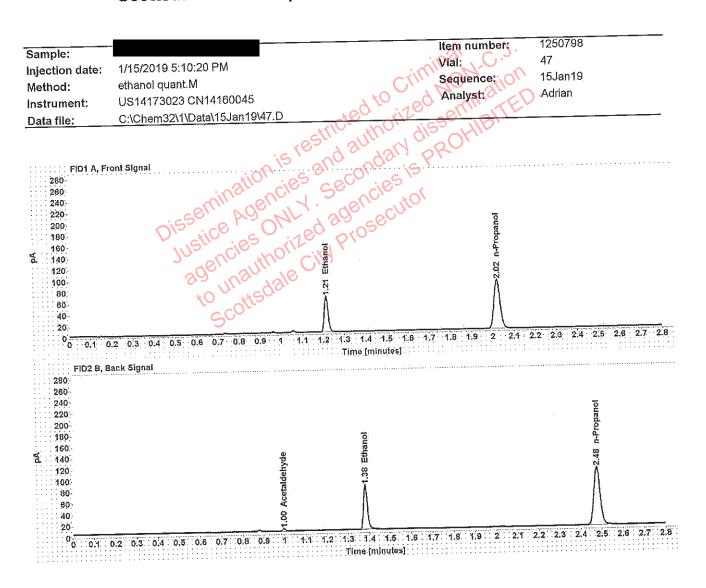


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,1223	1.213	82,404
n-Propanol		2.019	173.884

Compound	Time (min)	Peak Area
Acetaldehyde	0.997	4.153
Ethanol	1.382	101.266
n-Propanol	2.477	211.365

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

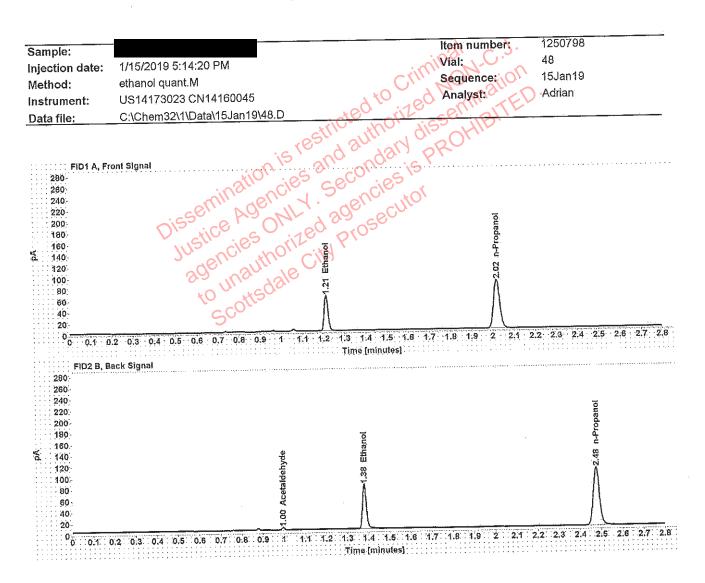

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1215	1.211	81.275
n-Propanol		2.017	172.687


#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.996	4.066
Ethanol	1.380	100.091
n-Propanol	2.475	210.120

User: wadrian 1/16/2019

#### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

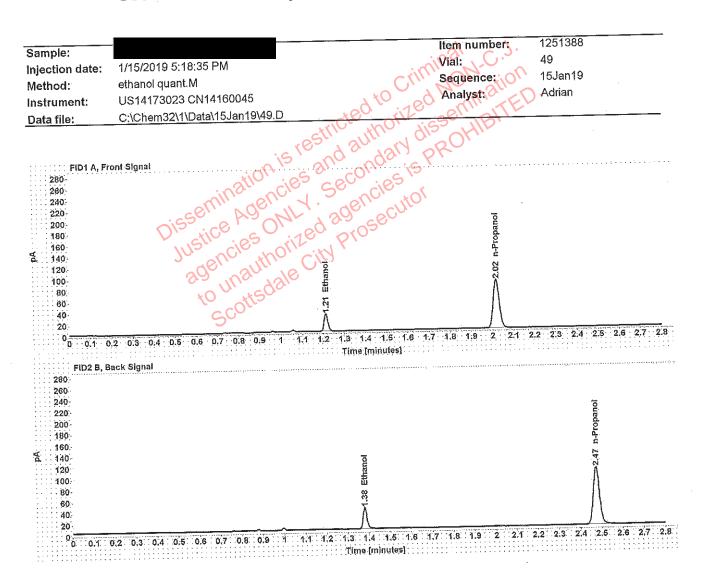


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0598	1.212	39,561
n-Propanol		2.017	171.532

Compound	Time (min)	Peak Area
Ethanol	1,380	48.215
n-Propanol	2.475	208.205

### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

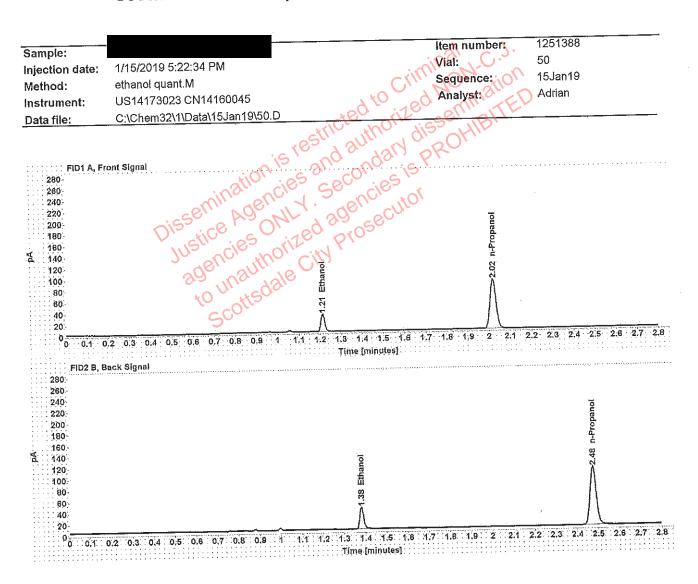

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0599	1,212	40.412
n-Propanol		2.018	175.004

Compound	Time (min)	Peak Area	
Ethanol	1,380	49,319	
n-Propanol	2.475	212.972	

# Scottsdale Police Department Crime Lab Volatiles Analysis

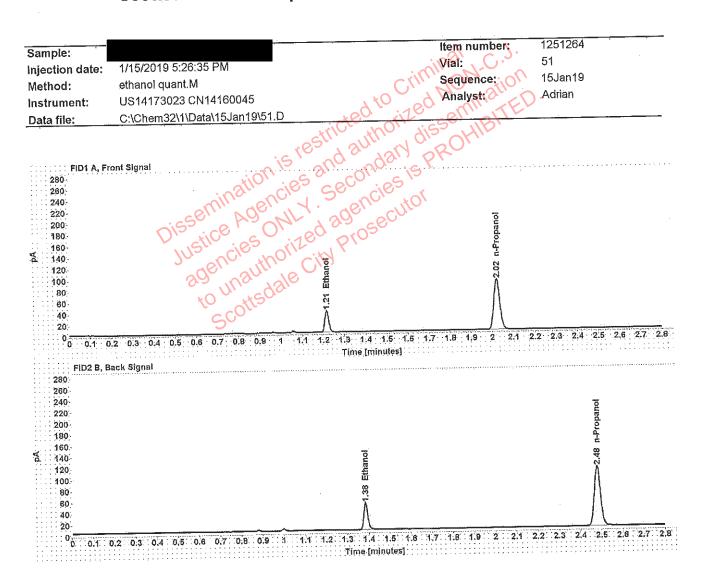


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0722	1.215	49.971
n-Propanol		2,021	179.329

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.385	61.085
n-Propanol	2.480	218.175

### Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

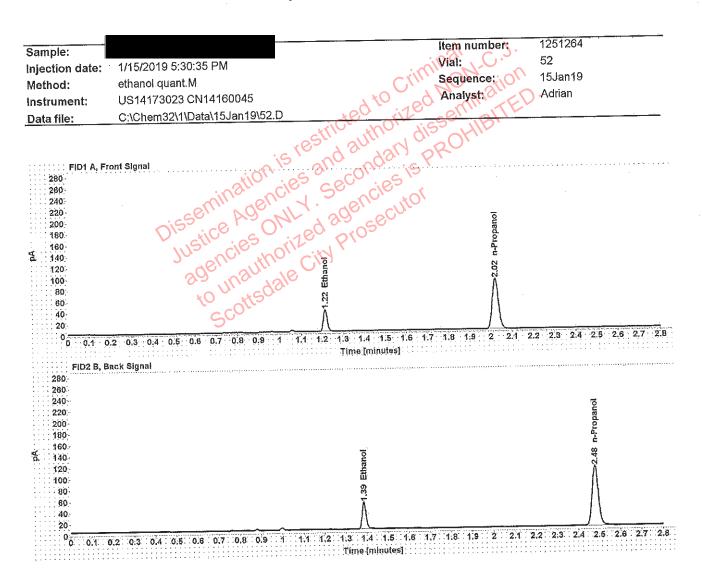

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0722	1.215	49.906
n-Propanol		2.021	178.947

Compound	Time (min)	Peak Area
Ethanol	1.385	61.045
n-Propanol	2.480	218.028

Case:

Scottsdale Police Department Crime Lab Volatiles Analysis

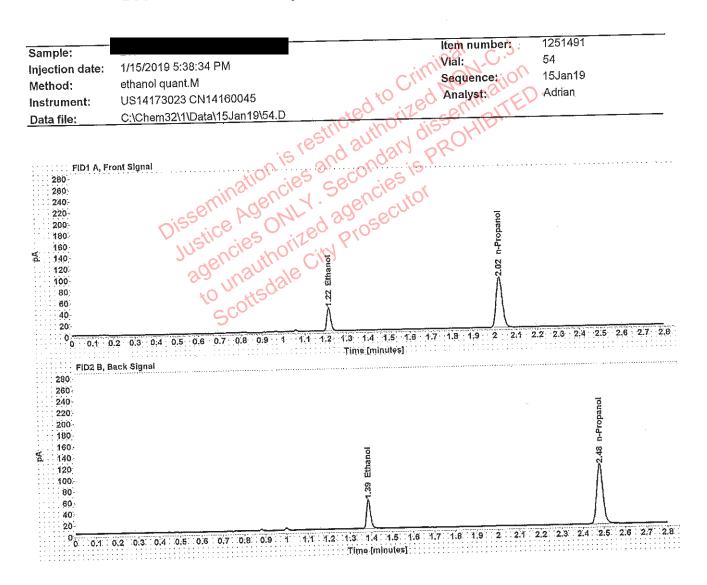


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0776	1,215	53,640
n-Propanol		2.021	178.803

Compound	Time (min)	Peak Area
Ethanol	1.386	65.603
n-Propanol	2.481	217.934

Case:

User: wadrian 1/16/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

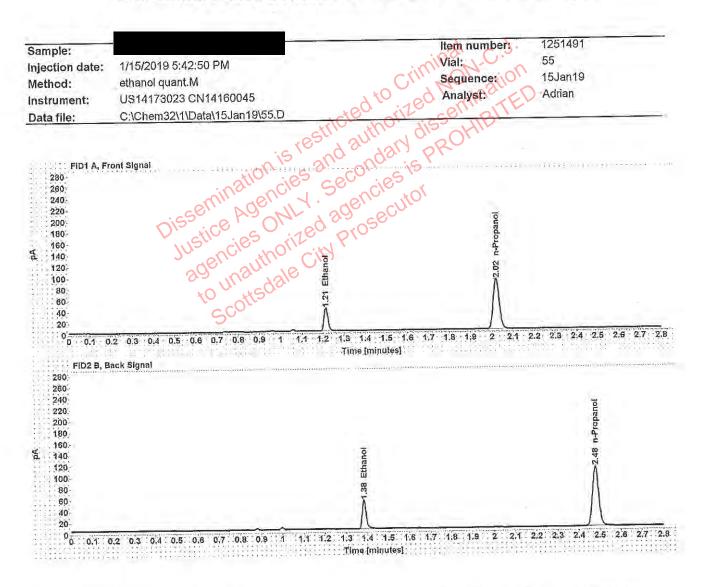


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0772	1.214	53,152
n-Propanol		2.020	178.160

Compound	Time (min)	Peak Area
Ethanol	1.384	64.922
n-Propanol	2.479	216.573

User: wadrian 1/16/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

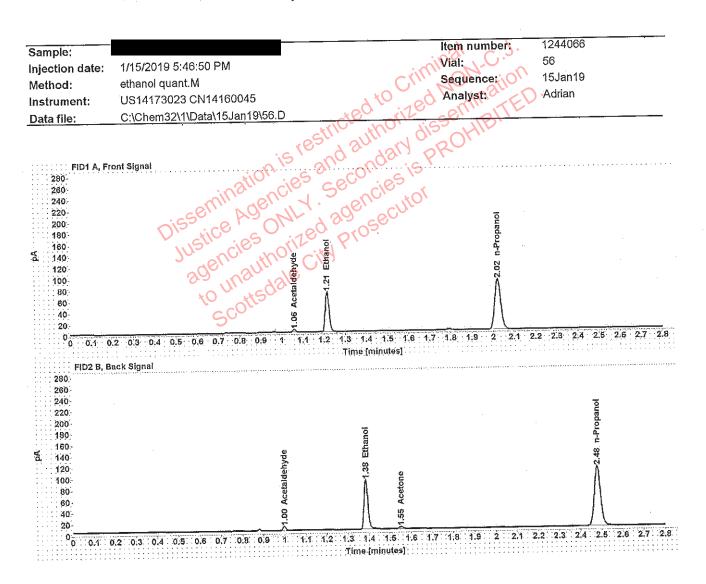


### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	5.055
>Ethanol	0.1327	1.214	91.947
n-Propanol		2,021	178.769

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	6.644
Ethanol	1.385	112.842
Acetone	1.551	4.257
n-Propanol	2.480	217.852

# Scottsdale Police Department Crime Lab Volatiles Analysis

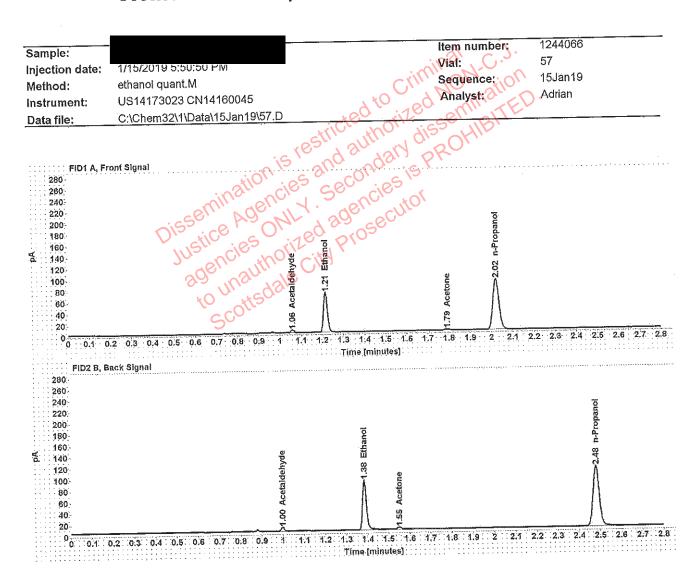

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	5,060
>Ethanol	0.1322	1.214	92.124
Acetone		1.791	3.754
n-Propanol		2.020	179.761

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	6.602
Ethanol	1.384	115.078
Acetone	1.550	4.998
n-Propanol	2.479	219,253

Case

### Scottsdale Police Department Crime Lab Volatiles Analysis

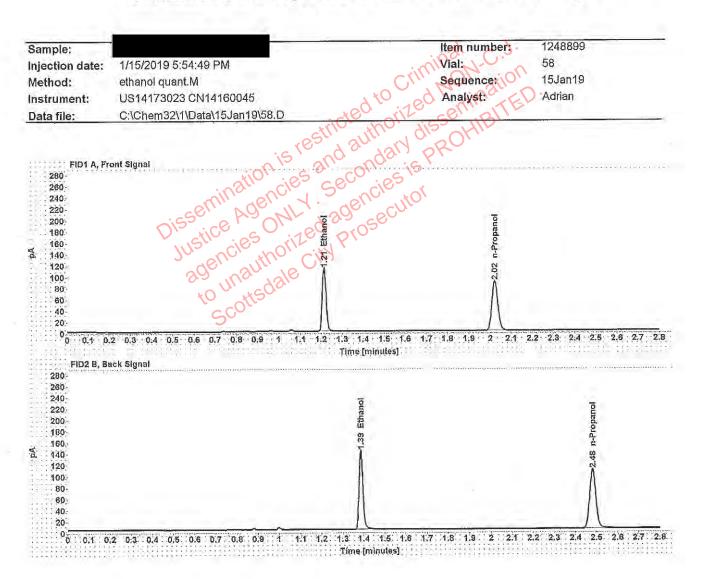


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2121	1.215	145.945
n-Propanol		2.021	177.180

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.386	180.195
n-Propanol	2.481	216,169

#### Case:

### Scottsdale Police Department Crime Lab Volatiles Analysis


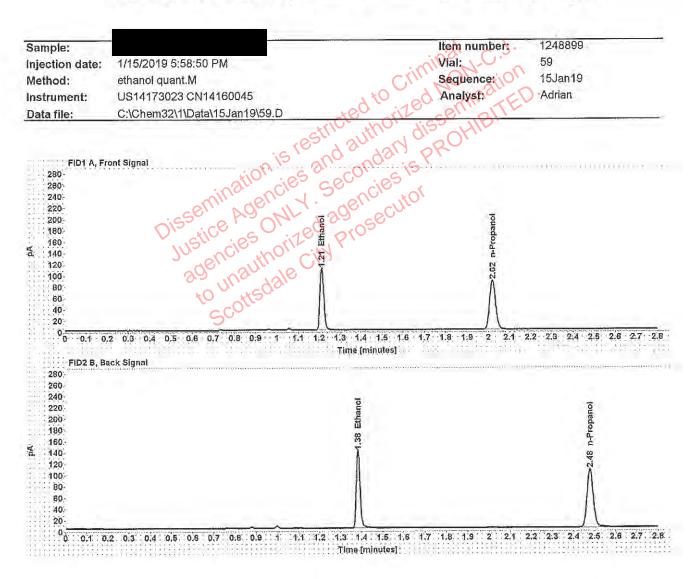


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2096	1.213	142.212
n-Propanol		2.020	174.792

Compound	Time (min)	Peak Area
Ethanol	1.383	175.694
n-Propanol	2.478	213.036

### Scottsdale Police Department Crime Lab Volatiles Analysis

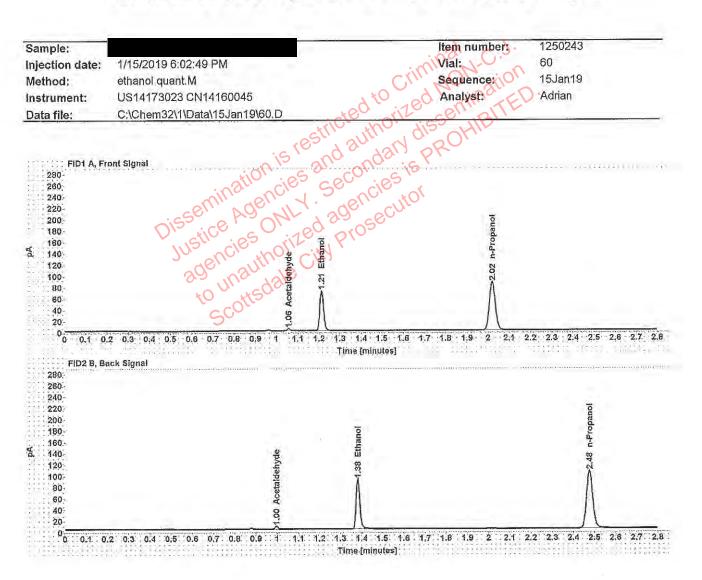


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.057	4.018
>Ethanol	0.1379	1.212	92.316
n-Propanol		2.019	172.680

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.996	5.229
Ethanol	1.381	113.549
n-Propanol	2.477	210.194

### Scottsdale Police Department Crime Lab Volatiles Analysis

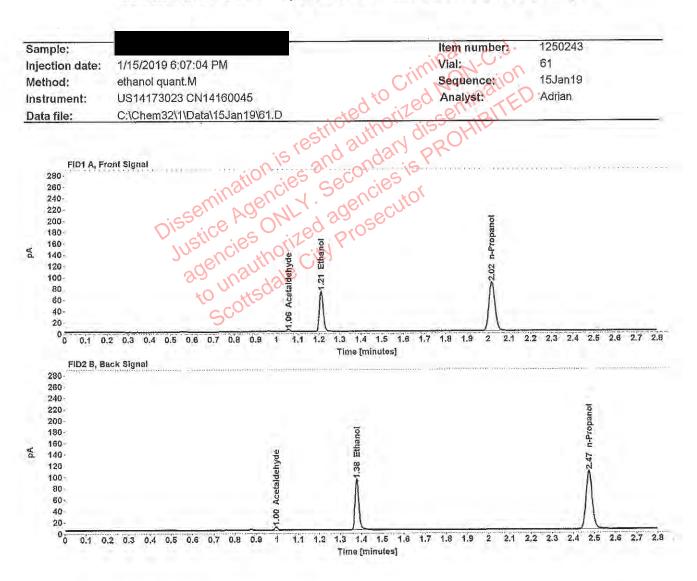


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.056	4.029
>Ethanol	0.1369	1.211	92.118
n-Propanol		2.017	173.532

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,995	5.268
Ethanol	1.378	112.975
n-Propanol	2.474	210.985

### Scottsdale Police Department Crime Lab Volatiles Analysis

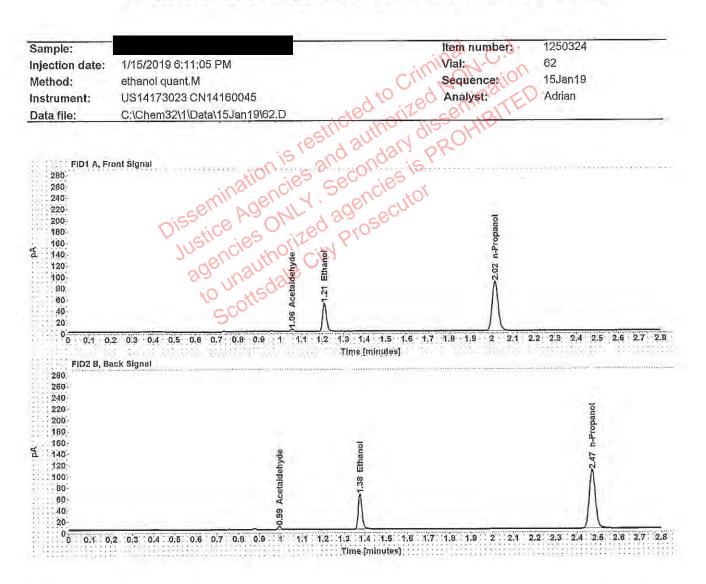

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.367
>Ethanol	0.0949	1,210	64.136
n-Propanol		2.016	174.734

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5,755
Ethanol	1.377	78,485
n-Propanol	2.472	212.890

### Scottsdale Police Department Crime Lab Volatiles Analysis

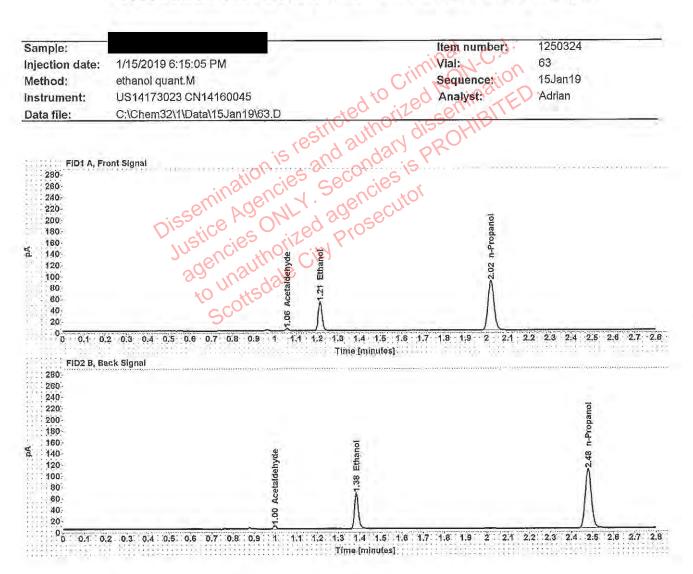



Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	4.328
>Ethanol	0.0973	1.214	66,736
n-Propanol		2.020	177.192

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	5.684
Ethanol	1.384	81,561
n-Propanol	2.479	216.101

### Scottsdale Police Department Crime Lab Volatiles Analysis

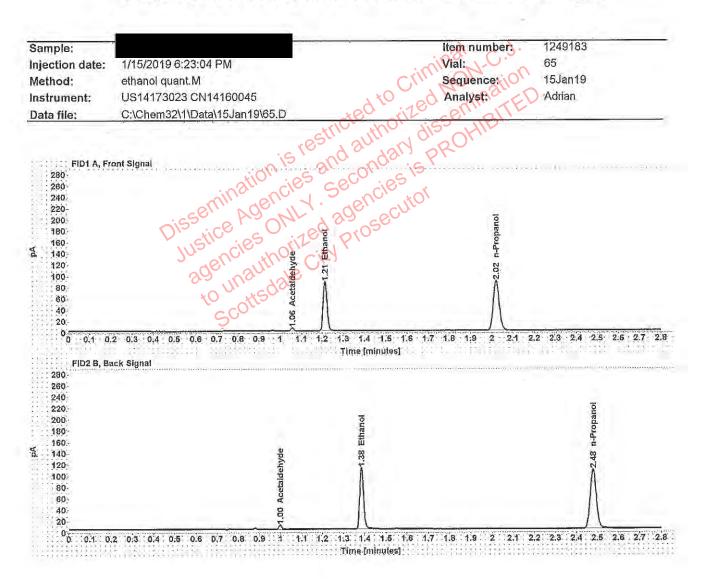


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1,058	5.438
>Ethanol	0.1652	1.214	113,354
n-Propanol		2.020	176,863

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	7.056
Ethanol	1.384	140,188
n-Propanol	2.479	216.028

### Scottsdale Police Department Crime Lab Volatiles Analysis

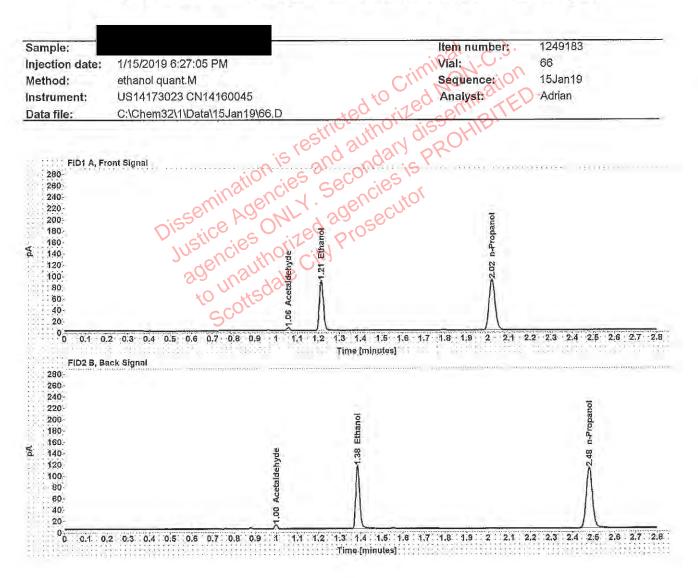

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.058	5.453
>Ethanol	0.1657	1.214	115.885
n-Propanol		2.021	180.240

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.998	7,115
Ethanol	1,384	143.369
n-Propanol	2.480	219.919

### Case:

### Scottsdale Police Department Crime Lab Volatiles Analysis

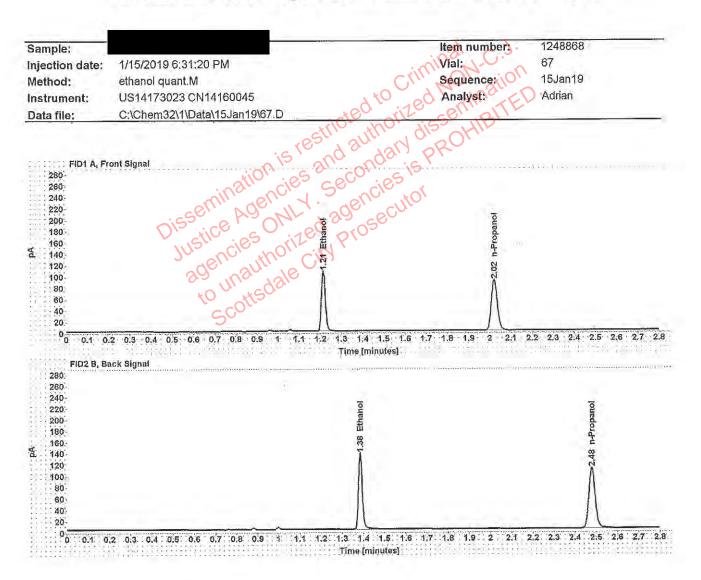


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1994	1.214	139.124
n-Propanol		2.021	179.724

Compound	Time (min)	Peak Area
Ethanol	1,385	173,588
n-Propanol	2.480	219,101

### Scottsdale Police Department Crime Lab Volatiles Analysis

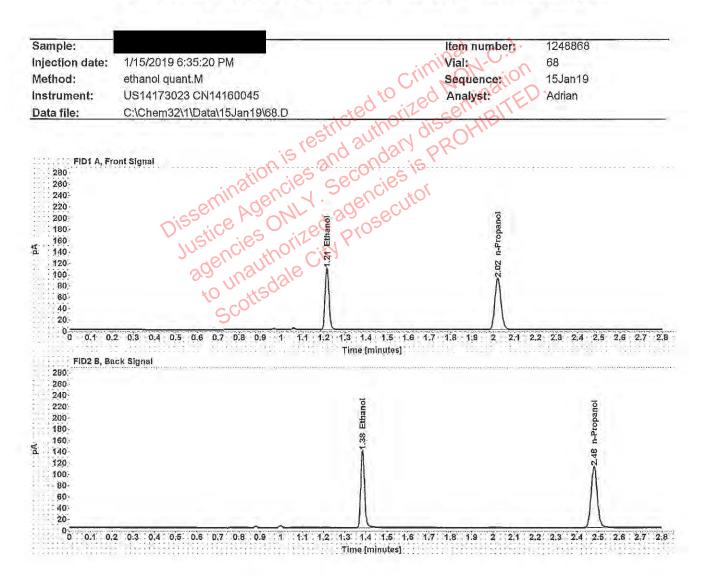


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2008	1.214	142.020
n-Propanol		2.021	182.208

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.384	177.597
n-Propanol	2,480	222,182