## SCOTTSDALE POLICE DEPARTMENT CRIME LABORATORY BLOOD ALCOHOL FACE SHEET

ANALYSIS DATE	04/17/2019	SEQUENCE NAME	17Apr19
EQUIPMENT Pipettor Gas Chromatograph	☐ Hamilton ML600 ☑ Agilent US14173		GJ10749
INSTRUMENT CAL	IBRATION	cito uthorn disso HIBN	
Vial 1 0.02 calibrator	Lot FN03241604	and any PR Coefficient o	f determination ( <b>r</b> ²)
Vial 2 0.10 calibrator	Lot FN06181501	2 <sup>CO</sup>	98
Vial 3 0.20 calibrator	Lot FN07201502	denc, cutor	
Vial 4 0.40 calibrator	of FN11191402	n OSE	
JUSC	encie uthoricity	K	

## CALIBRATION VERIFICATION AND RESOLUTION TEST

Vial	Sample	Expected result	Measured result	Manufacturer/lot
5	Blank	Not detected	Not detected	SPD lab 121118
6	Volatiles mixture	6 compounds	6 compounds	SPD lab 020917WLA
7	Aqueous control	0.400 g/dL	0.400 g/dL	Lipomed 08012015-C
8	Aqueous control	0.040 g/dL	0.039 g/dL	Lipomed 09022015-A
9	Blood control	0.198 g/dL	0.197 g/dL	ACQ 407041529/13
20	Aqueous control	0.080 g/dL	0.080 g/dL	Lipomed 28082014-B
31	Aqueous control	0.150 g/dL	0.152 g/dL	Lipomed 09022015-C
42	Blood control	0.198 g/dL	0.200 g/dL	ACQ 407041529/13
53	Aqueous control	0,080 g/dL	0.081 g/dL	Lipomed 28082014-B
62	Aqueous control	0.400 g/dL	0.404 g/dL	Lipomed 08012015-C
63	Aqueous control	0.040 g/dL	0.040 g/dL	Lipomed 09022015-A
64	Blood control	0.198 g/dL	0.200 g/dL	ACQ 407041529/13
65	Blank	Not detected	Not detected	SPD lab 121118

#### SUBJECT SAMPLES

Subjects in the sequence \_\_\_\_\_24\_\_\_\_

Subjects requiring reanalysis \_\_\_\_1

ADDITIONAL NOTES: Position 12/13 (DR 19-06442) duplicates exceeded the acceptable range of 2% difference from the mean and will therefore be reanalyzed.

Run valid Analyst Run valid Run valid Run invalid Analyst Run invalid Technical Reviewer

Document ID: **1208** Revision Date:02/27/2017 Issuing Authority: Kris Cano, Forensic Services Director Page 1 of 1


# Scottsdale Police Department Crime Laboratory Sequence Quality Assurance Summary


#### SEQUENCE NAME: 17Apr19

#### ANALYST: Adrian

Sample Name	Vial	Measured Value (g/dL)	Expected Value (g/dL)	Percent Difference	Absolute Difference (g/dL)
blank 121118	5	negative	negative	1.0.	-
0.400 08012015-C	7	0.400	0.400	0.00	0.000
0.040 09022015-A	8	0.039	0.040	2.50	-0.001
0.198 407041529/13	9	0.197 👡 🖉	0.198	0.51	-0.001
0.080 28082014-B	20	0.080	v00.080	0.00	0.000
0.150 09022015-C	31	0,152	0.150	1.33	0.002
0.198 407041529/13	42	S 0.200	200.198	1.01	0.002
0.080 28082014-B	53	0.081	0.080	1.25	0.001
0.40 08012015-C	62	0.404	0.400	1.00	0.004
0.04 09022015-A	63	0.040	0.040	0.00	0.000
0.198 407041529/13	64	0.200	0.198	1.01	0.002
blank 121118	65	O negative	negative	-	_

JUST PROPERTY NONL	-ity F		
Calibrator	Ethanol Area	N-propanol Area	Ratio
0.020	11.933	162.040	0.074
0.100	61.676	164.466	0.375
0.200	124.830	164.910	0.757
0.400	252.885	165.622	1,527

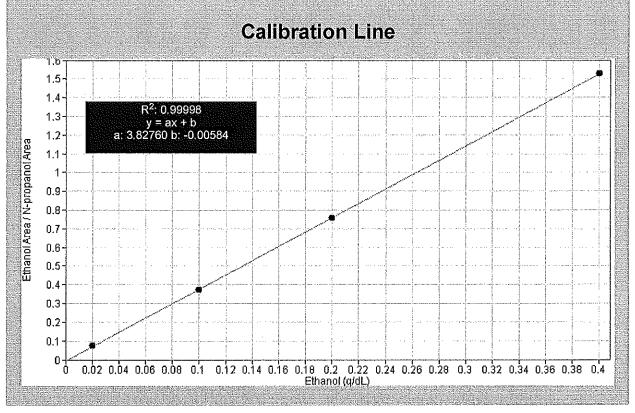


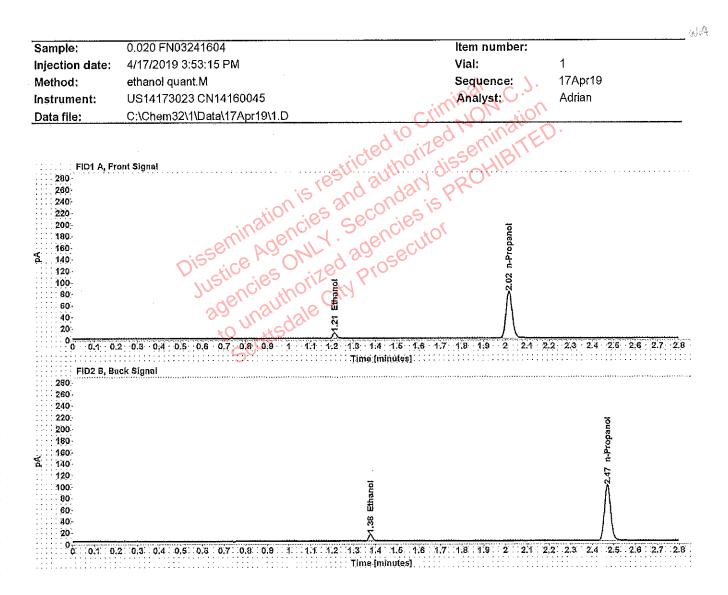

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.212	11.933
n-Propanol	2,016	162.040


Compound	Time (min)	Peak Area
Ethanol	1.376	14.728
n-Propanol	2.470	197.208

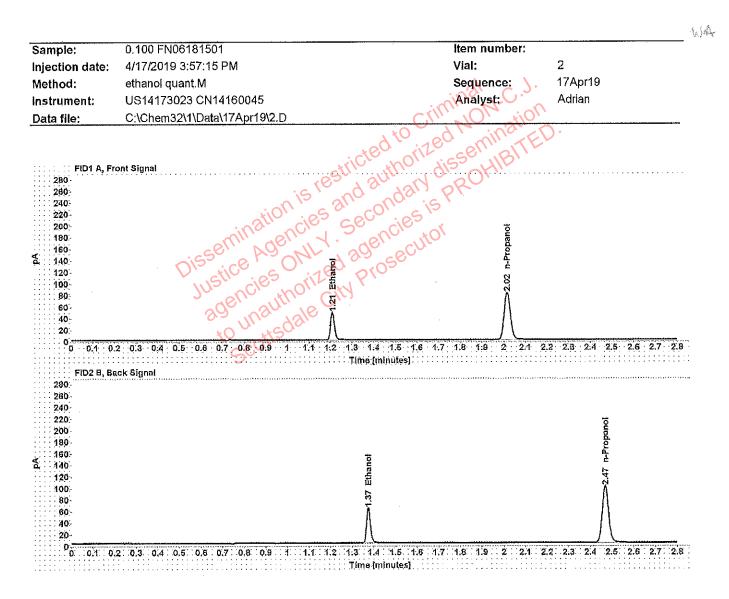

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.209	61.676
n-Propanol	2,015	164.466

Compound	Time (min)	Peak Area
Ethanol	1.374	76.512
n-Propanol	2.470	200,766

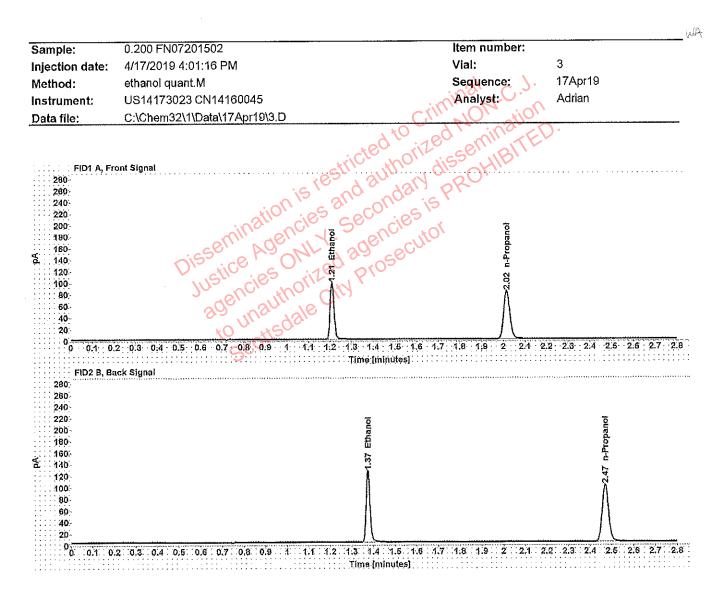


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.209	124.830
n-Propanoi	2,016	164.910

Compound	Time (min)	Peak Area
Ethanol	1.374	155.281
n-Propanol	2.470	201.656




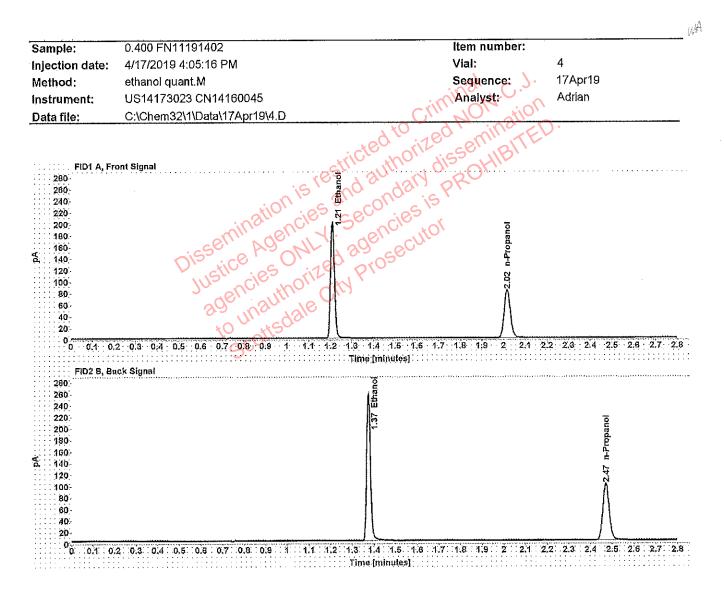

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.208	252,885
n-Propanol	2,016	165.622

Compound	Time (min)	Peak Area
Ethanol	1.374	315.880
n-Propanol	2.471	202.553

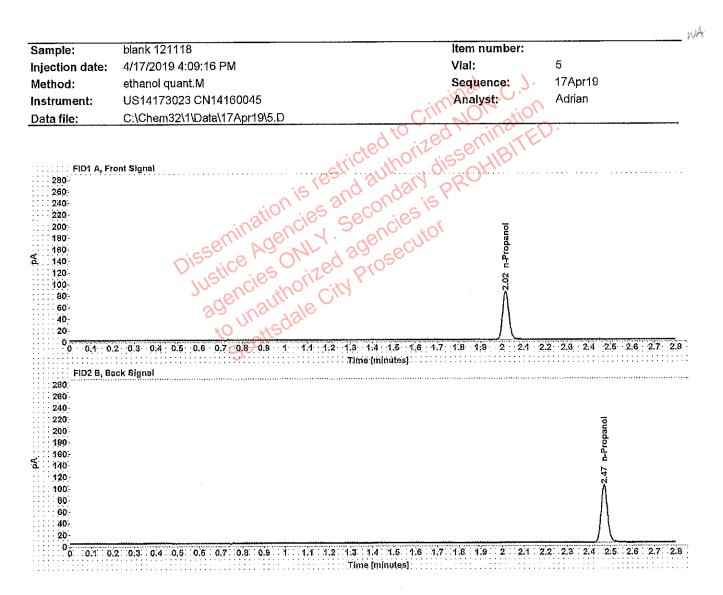


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.015	166.852

Compound	Time (min)	Peak Area
n-Propanol	2.470	203.517




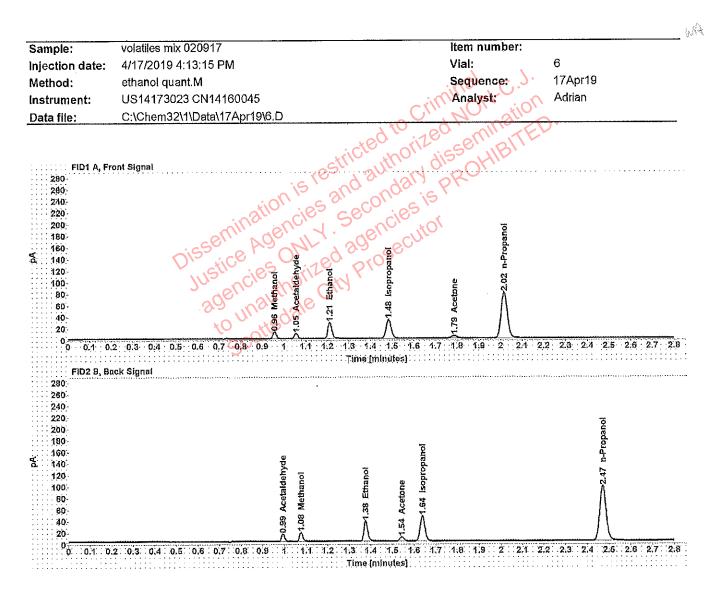

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Methanol		0,957	13,051
Acetaldehyde		1.055	9.866
>Ethanol	0.0603	1.210	35,812
Isopropanol		1.484	52.739
Acetone		1.786	7.714
n-Propanol	Pano 70	2.016	159.279


Compound	Time (min)	Peak Area
Acetaldehyde	0.992	12.743
Methanol	1,076	16,608
Ethanol	1.376	44.285
Acetone	1.544	9.184
Isopropanol	1.638	66,158
n-Propanol	2.471	194.237

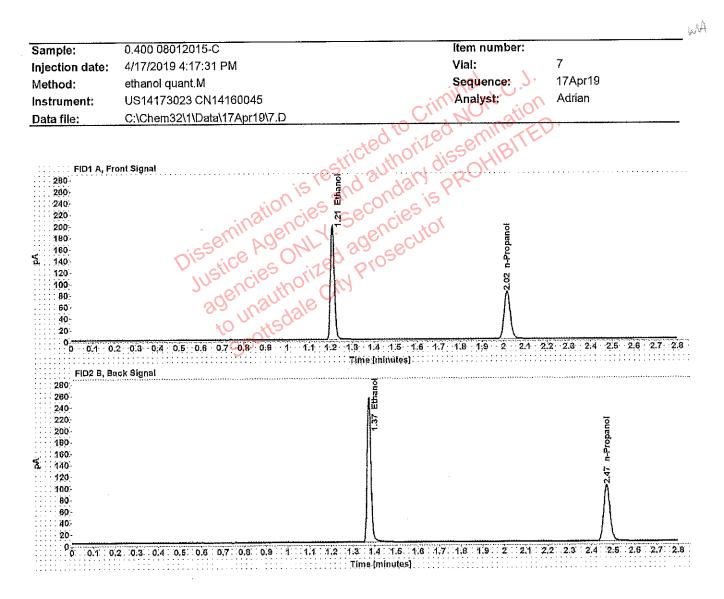

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.4007	1.208	249.900
n-Propanol		2,016	163.551


Compound	Time (min)	Peak Area
Ethanol	1.374	312.105
n-Propanol	2.470	199.791

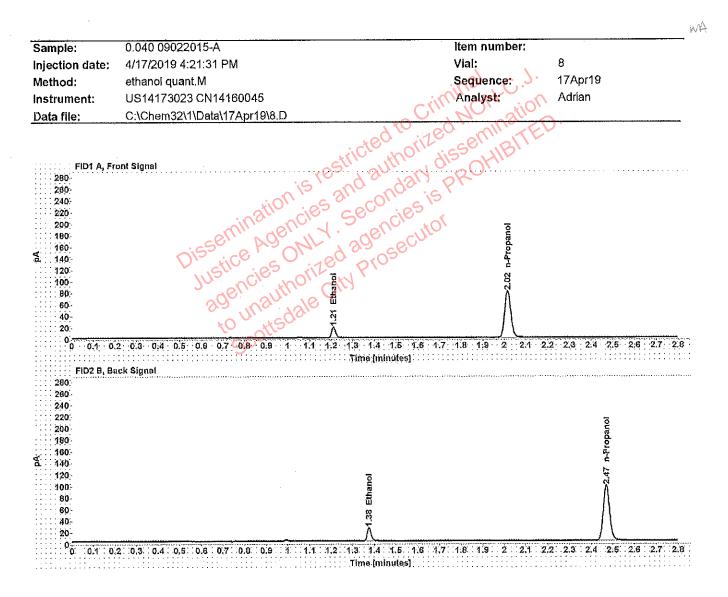

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,0399	1.210	23,542
n-Propanol		2.015	160.201


Compound	Time (min)	Peak Area
Ethanol	1.375	29.055
n-Propanol	2.470	195.564

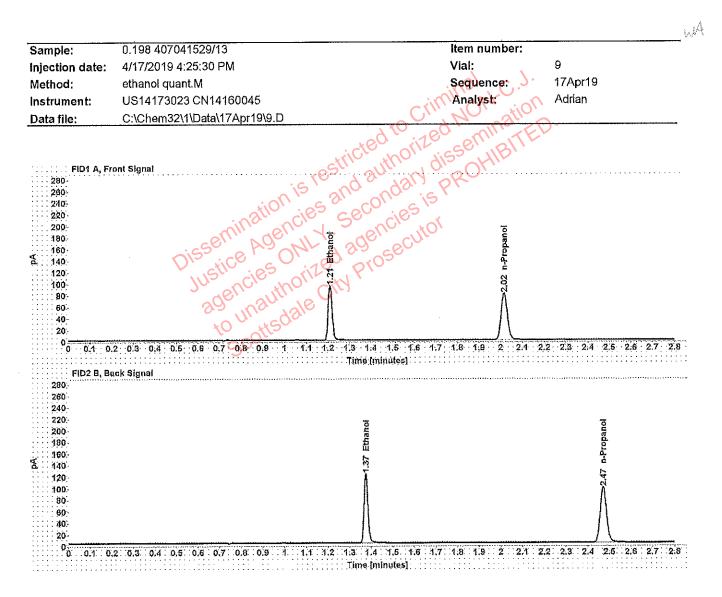

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1975	1.209	121.074
n-Propanol		2.016	161.393


Compound	Time (min)	Peak Area
Ethanol	1.375	150.952
n-Propanol	2.471	196.933

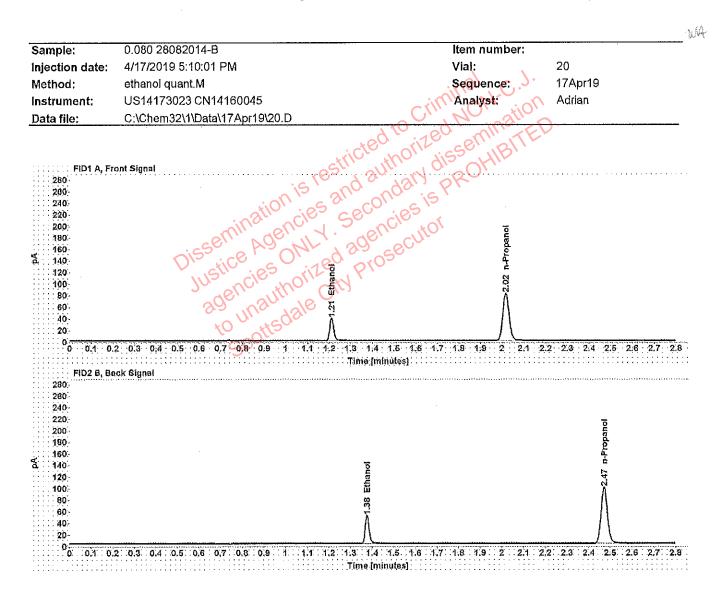

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	8080,0	1.210	49.292
n-Propanol		2.016	162.494


Compound	Time (min)	Peak Area
Ethanol	1.376	60.946
n-Propanol	2.472	198,188

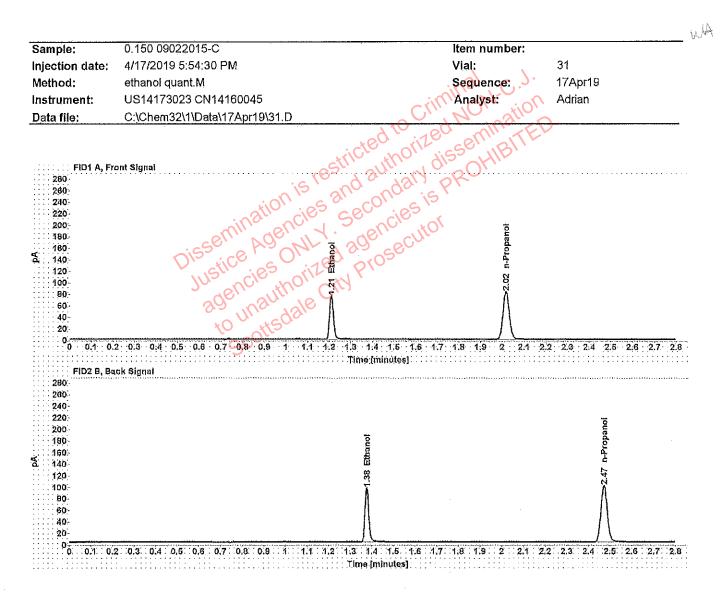

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1525	1.210	95.544
n-Propanol		2,016	165.339


Compound	Time (min)	Peak Area
Ethanol	1.376	119.014
n-Propanol	2.472	201,949

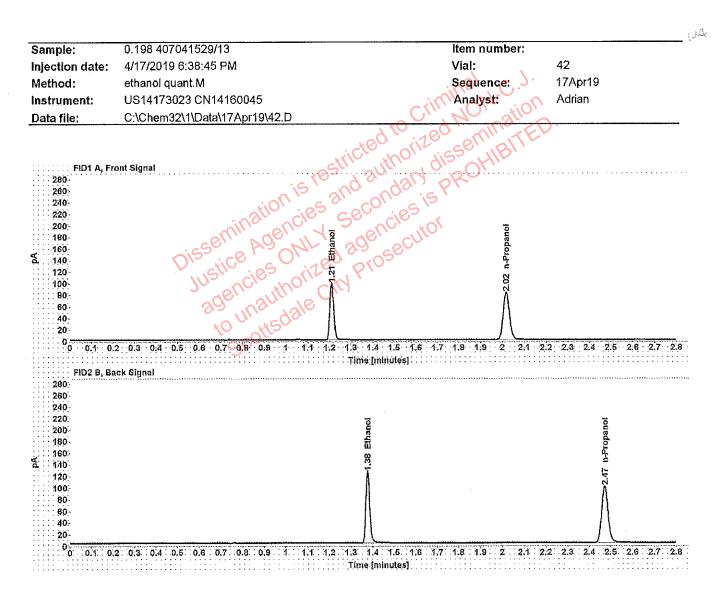

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,2005	1,210	124.321
n-Propanol		2.017	163.209


Compound	Time (min)	Peak Area
Ethanol	1.376	155.145
n-Propanol	2.472	199.833

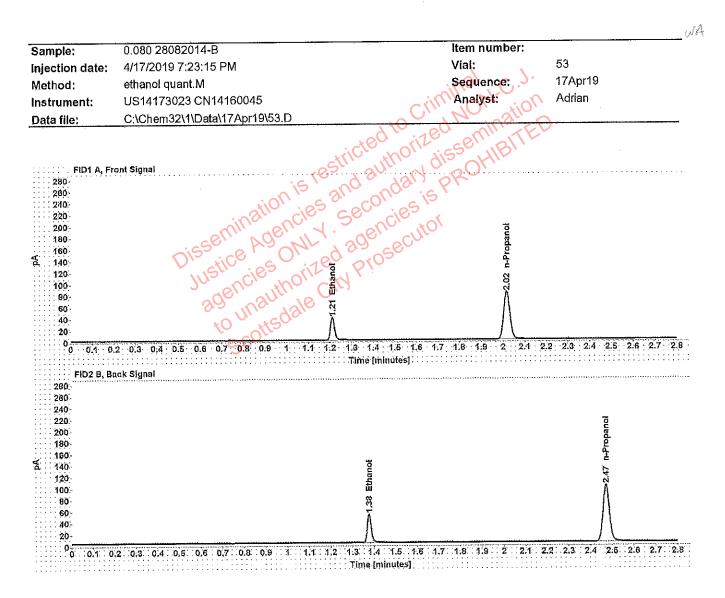

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0814	1.210	50.443
n-Propanol	Junon	2,016	164.908


Compound	Time (min)	Peak Area
Ethanol	1.376	62.563
n-Propanol	2.472	201.670

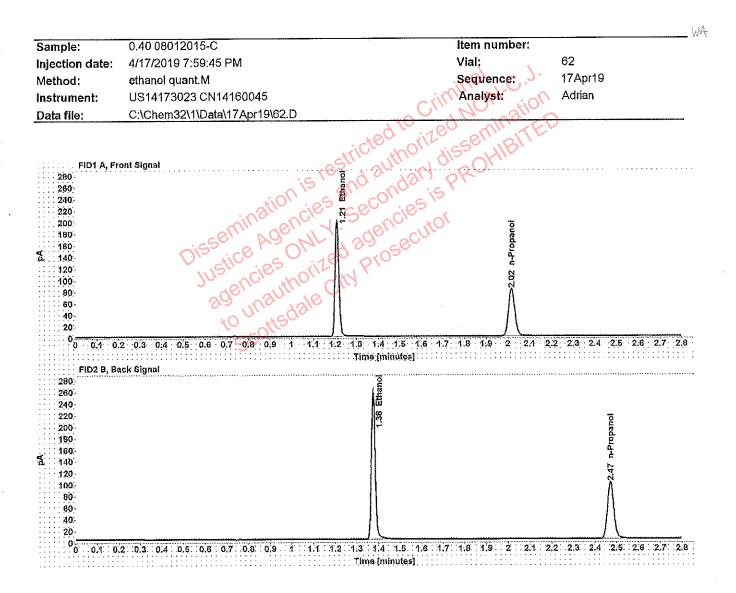

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.4045	1,209	252,061
n-Propanol	*-#***	2,016	163.419


Compound	Time (min)	Peak Area
Ethanol	1.375	316,008
n-Propanol	2,471	200,477

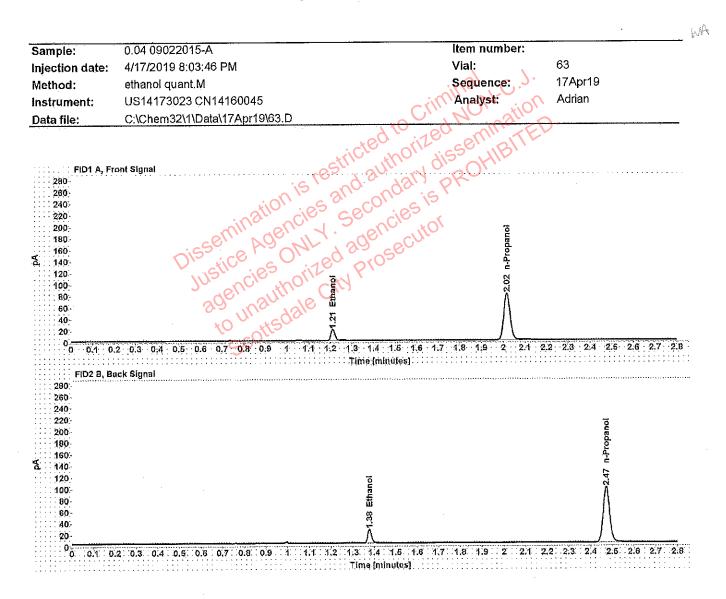

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0406	1.211	24.162
n-Propanol		2,016	161.547


Compound	Time (min)	Peak Area
Ethanol	1.377	29.909
n-Propanol	2.472	197.612

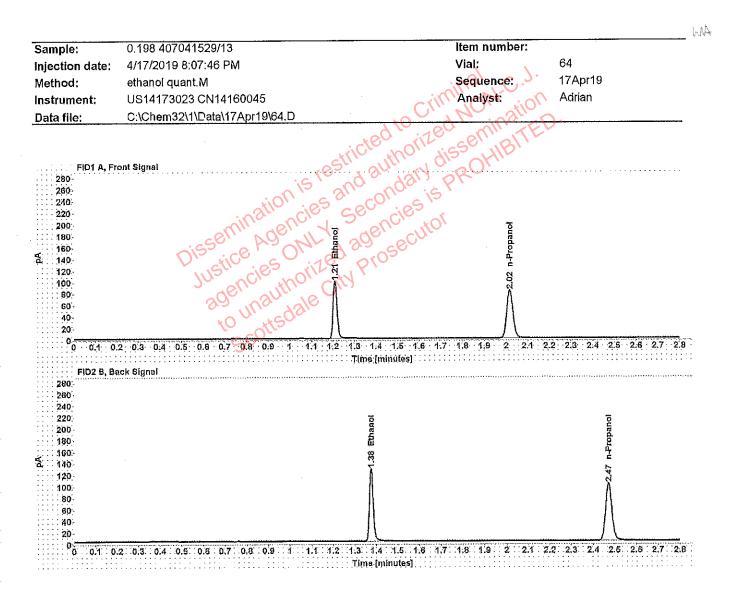

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2001	1.209	126.555
n-Propanol		2.016	166.497

Compound	Time (min)	Peak Area
Ethanol	1.376	158,272
n-Propanol	2.471	203,905

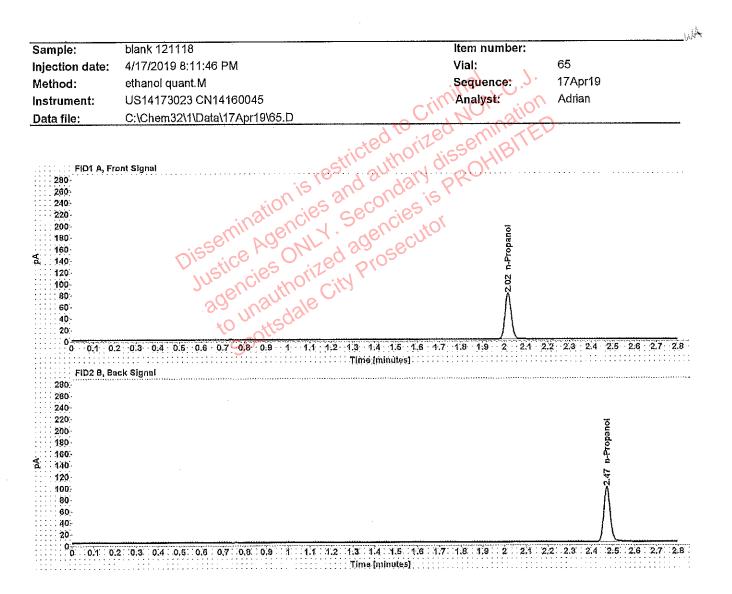

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2,016	159,611

Compound	Time (min)	Peak Area
n-Propanol	2.472	195.436

#### Sequence Summary

Page 1 of 2

Analyst: Adrian Instrument: US14173023 CN14160045 Sequence name: 17Apr19 Method Item Number Vial Sample Type ethanol quant.M 0.020 FN03241604 Calibration 1 ethanol guant.M Calibration 2 0.100 FN06181501 ethanol quant.M 0.200 FN07201502 Calibration 3 Calibration ethanol guant.M 4 0.400 FN11191402 Control ethanol quant.M 5 blank 121118 ethanol quant.M Control 6 volatiles mix 020917 Control ethanol quant.M 0.400 08012015-C 7 Control ethanol quant.M 8 0.040 09022015-A ethanol quant.M 9 0,198 407041529/13 Control 1259507 ethanol quant.M 10 Sample ethanol quant.M 1259507 Sample 11 12 Sample 1264044 ethanol quant.M 1264044 ethanol quant.M 13 Sample 1260752 ethanol quant.M Sample 14 1260752 ethanol guant.M Sample 15 Sample 1260771 ethanol guant.M 16 1260771 ethanol quant.M 17 Sample ethanol quant.M 1260703 18 Sample Sample 1260703 ethanol quant.M 19 ethanol quant.M 20 0.080 28082014-B Control 1259744 ethanol quant.M 21 Sample Sample 1259744 ethanol quant.M 22 23 Sample 1261550 ethanol quant.M 1261550 ethanol quant.M 24 Sample 1238318 ethanol quant.M Sample 25 1238318 ethanol quant.M Sample 26 Sample 1264587 ethanol quant.M 27 1264587 ethanol quant.M 28 Sample 1264886 ethanol quant.M Sample 29 1264886 ethanol quant.M 30 Sample 31 0.150 09022015-C Control ethanol quant.M 176-01A ethanol quant.M Sample 32 176-01A ethanol quant.M Sample 33 Sample 176-01A ethanol quant.M 34 176-01A ethanol guant.M 35 Sample ethanol guant.M 1264726 Sample 36 37 Sample 1264726 ethanol guant.M 1261928 ethanol quant.M 38 Sample 1261928 ethanol quant.M Sample 39 Sample 1261921 ethanol quant.M 40 1261921 ethanol quant.M Sample 41 0.198 407041529/13 Control ethanol quant.M 42 1262626 ethanol quant.M Sample 43 1262626 ethanol quant.M Sample 44 1243213 ethanol quant.M 45 Sample Sample 1243213 ethanol quant.M 46 ethanol quant.M 1261683 47 Sample

W

## Sequence Summary

	(7A)	19 JABIST	द	Page 2 of 2
48		Sample	1261683	ethanol quant.M
49		Sample	1262294	ethanol quant.M
50		Sample 🔬	1262294	ethanol quant.M
51		Sample (\\\	1262927	ethanol quant.M
52		Sample	1262927	<ul> <li>ethanoi quant.M</li> </ul>
53	0.080 28082014-B	Control	ente	ethanol quant.M
54	1114-	Sample	1262981	ethanol quant.M
55	(C)	Sample	1262981	ethanol quant.M
56		Sample	1262799	ethanol quant.M
57	ation's es	CO Sample	1262799	ethanol guant.M
58		Sample	1263017	ethanol quant.M
59	CON, NOR IN .	Sample	1263017	ethanol quant.M
60		Sample	1263401	ethanol quant.M
61	LISTIC CIES ON LE	Sample	1263401	ethanol quant.M
62	0.40 08012015-C	Control		ethanol quant.M
63	0.04 09022015-A	Control		ethanol quant.M
64	0.198 407041529/13 0 0 00 000	Control		ethanol guant.M
65	blank 121118	Control		ethanol quant.M

# Scottsdale Police Department Crime Laboratory Summary of Cases

SEQUEN	CE NAME: 17Apr19			al Cu	ANALYST: Adrian
Vials	Test 1 (g/dL)	Test 2 (g/dL)	Mean (g/dL)	Percent Difference*	Difference (g/dL)*
10 11	0.1755	0.1761	0.17580	0.17	0.00030
12 13	0.1831	0.1921	0.18760	2.40	0.00450
14 15	0,1617	0.1624	0.16205	······································	0.00035
16 17	0.1940	0,1956 🦯	0,19480	0.41	0.00080
18 19	0.1451	0.1471	0.14610	0.68	0.00100
21 22	0.3040	0.3042	0.30410	0.03	0.00010
23 24	0.1774	0.1770 5	0,17720	0.11	0.00020
25 26	0.1839	0.1859	C 0.18490	0.54	0.00100
27 28	0.1003	0.1002	0,10025	0.05	0.00005
29 30	0.1651 5	0.1655	0.16530	0.12	0.00020
32 33	0.2605	0.2593	0,25990	0.23	0.00060
34 35	0,1328	0.1322	0.13250	0.23	0.00030
36 37	0.2191	0.2184	0,21875	0.16	0,00035
38 39	0.1856	0,1865	0,18605	0.24	0.00045
40 41	0.2252	0.2257	0,22545	0.11	0.00025
43 44	0.1200	0,1200	0.12000	0.00	0.00000
45 46	0.1296	0.1286	0.12910	0.39	0.00050
47 48	0.2441	0.2419	0.24300	0.45	0.00110
49 50	0.1891	0,1897	0.18940	0.16	0.00030
51 52	0.1888	0.1869	0.18785	0.51	0.00095
54 55	0.2605	0.2607	0.26060	0.04	0.00010
56 57	0,2506	0,2522	0.25140	0.32	0.00080
58 59	0,2224	0,2232	0.22280	0.18	0.00040
60 61	0.1051	0.1056	0.10535	0.24	0.00025

\*Calculated differences are differences from the mean of the two results.

## : Adrian, William - (18-Apr-2019)

User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

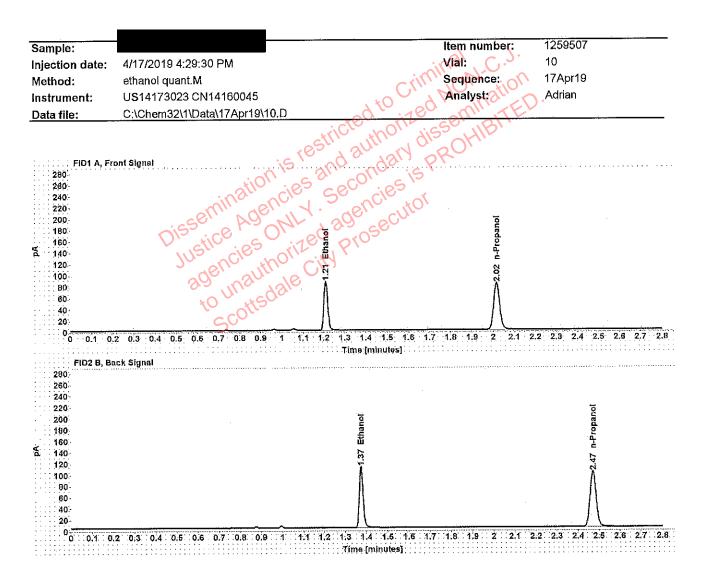


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1755	1.209	110.607
n-Propanol		2,016	166.067


Compound	Time (min)	Peak Area
Ethanol	1.375	137.166
n-Propanol	2,471	202.578

### Adrian, William - (18-Apr-2019)

Case:

User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

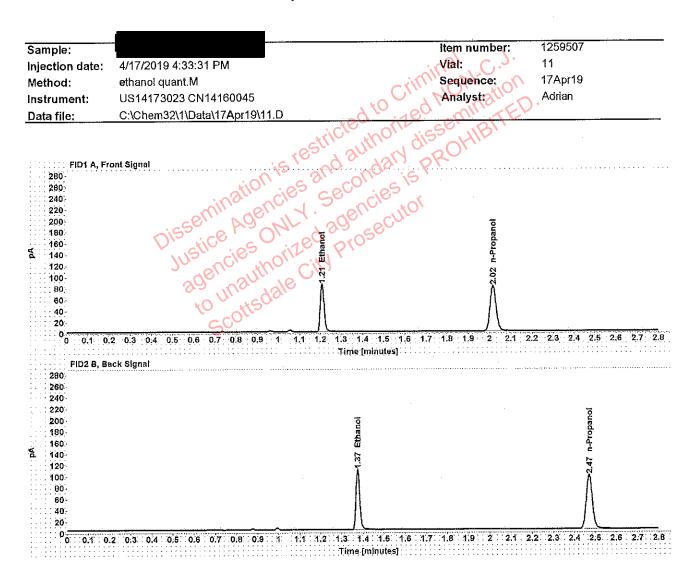

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1761	1.209	107.862
n-Propanol	<b>FN</b>	2.016	161.383

Compound	Time (min)	Peak Area
Ethanol	1.375	134.094
n-Propanol	2.471	196.844

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

Case:

## Scottsdale Police Department Crime Lab Volatiles Analysis

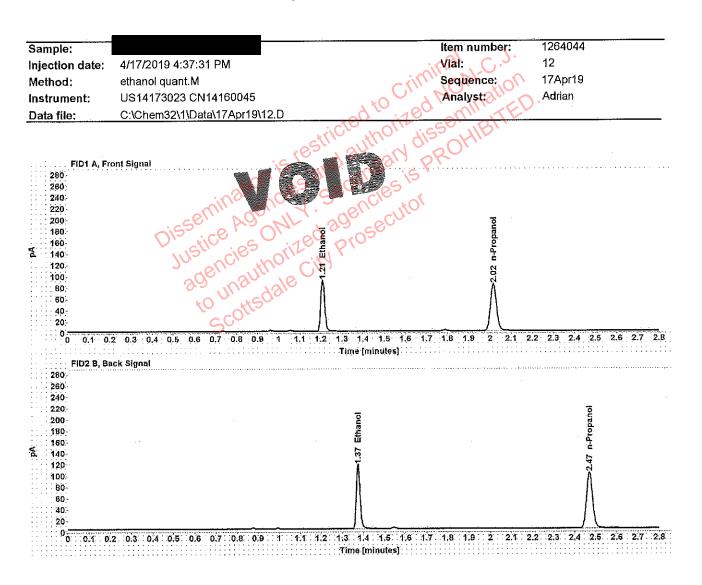



Table 1: FID 1 A (	column DB-ALC1)
--------------------	-----------------

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1831	1.209	116.041
n-Propanol		2,016	166.927

Compound	Time (min)	Peak Area
Ethanol	1.374	144.106
n-Propanol	2.470	204.842

## Case:

## Scottsdale Police Department Crime Lab Volatiles Analysis

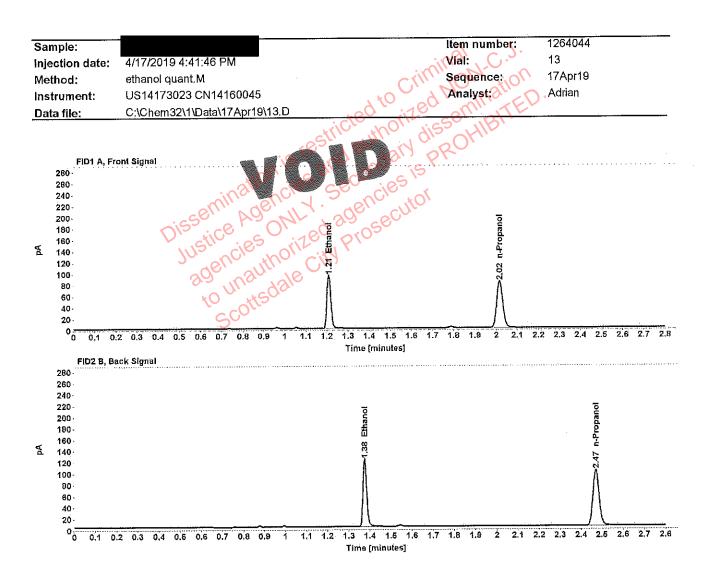

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1921	1,209	120.768
n-Propanol		2.016	165.580

Compound	Time (min)	Peak Area
Ethanol	1.375	150.562
n-Propanol	2.471	203.057

# Adrian, William - (18-Apr-2019)

User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

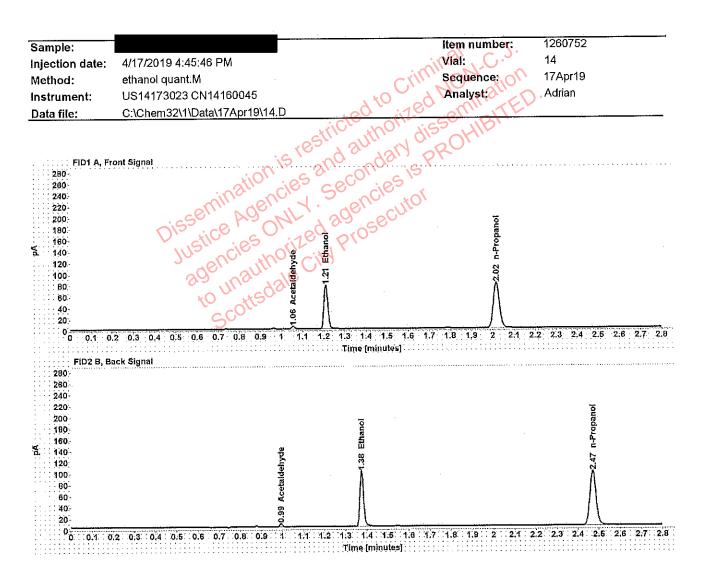


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4,323
>Ethanol	0.1617	1.209	99.244
n-Propanol	ua para n	2,016	161.858

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	5.646
Ethanol	1,375	122.805
n-Propanol	2.471	197.718

### : Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

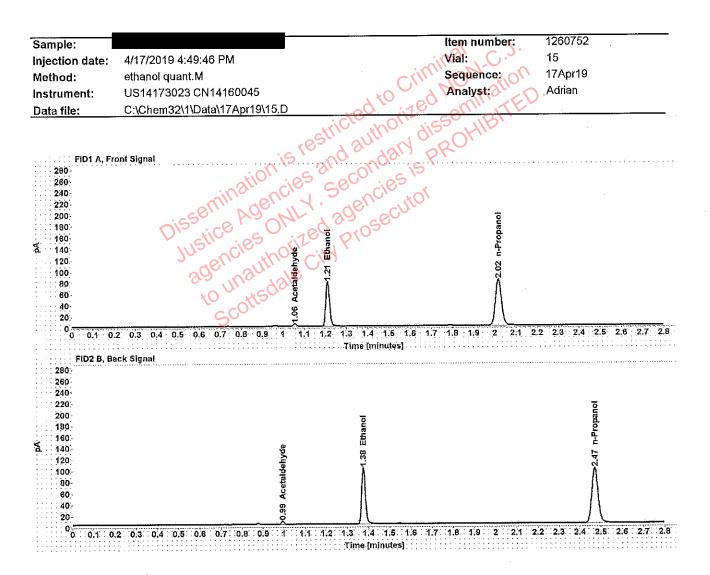

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.289
>Ethanol	0.1624	1.210	100,512
n-Propanol		2.016	163.203

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,993	5.616
Ethanol	1.375	124.367
n-Propanol	2.471	199.131

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

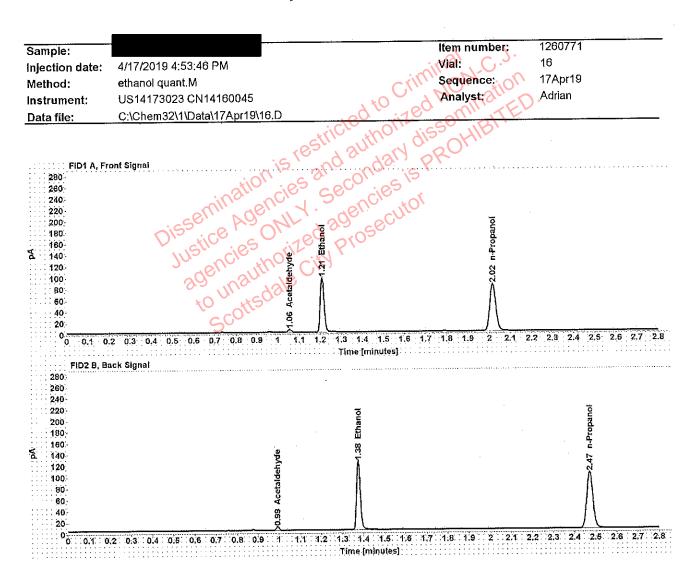


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	5.164
>Ethanol	0.1940	1,209	123.019
n-Propanol		2.016	166.982


#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,993	6.741
Ethanol	1.375	153.288
n-Propanol	2.471	204.082

### : Adrian, William - (18-Apr-2019)

User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

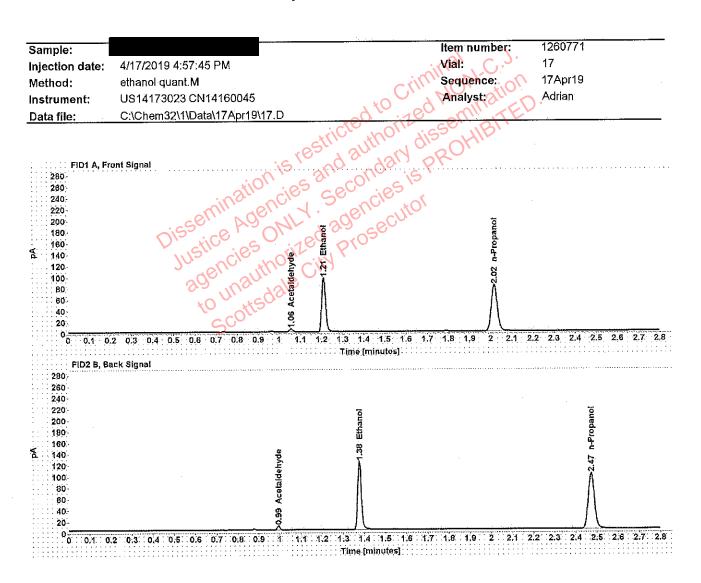

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde	LIVARD	1.055	5.266
>Ethanol	0.1956	1.210	122.643
n-Propanol		2.016	165.138

#### Table 2: FID 2 B (column DB-ALC2)


Compound	Time (min)	Peak Area
Acetaldehyde	0.994	6.892
Ethanol	1,376	152.830
n-Propanol	2.472	201.676

## Adrian, William - (18-Apr-2019)

Case:

User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

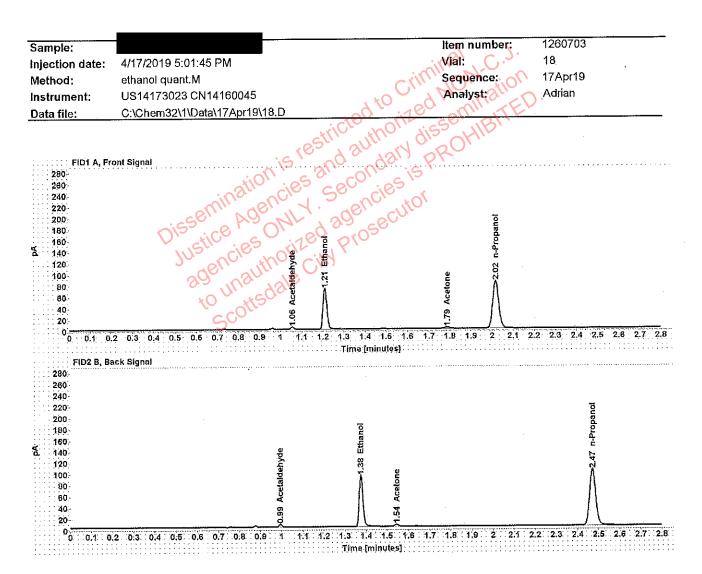

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	3.882
>Ethanol	0.1451	1.209	92.420
Acetone		1.787	4.032
n-Propanol		2.016	168.221

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	5.089
Ethanol	1.375	114.041
Acetone	1.544	4.724
n-Propanol	2,471	205.215

# Adrian, William - (18-Apr-2019)

#### User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

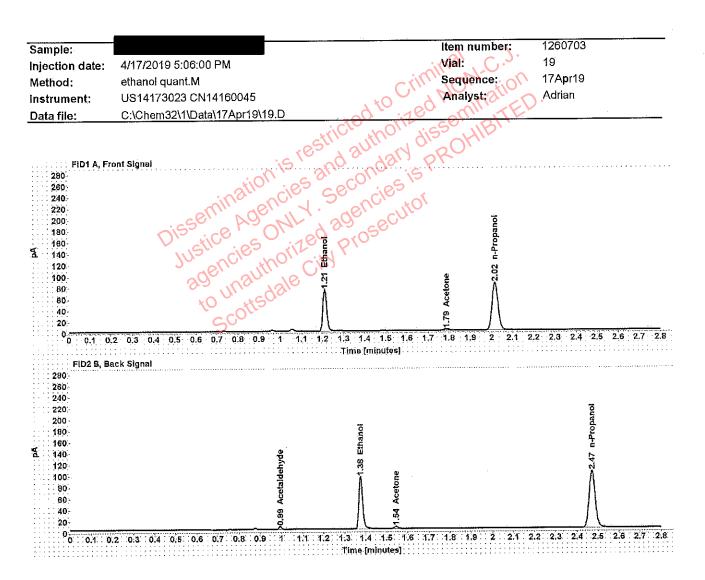


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1471	1.210	94,024
Acetone		1.787	4,060
n-Propanol		2.016	16B.715

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.774
Ethanol	1.376	116.239
Acetone	1,545	4.732
n-Propanol	2.472	205,481

### : Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

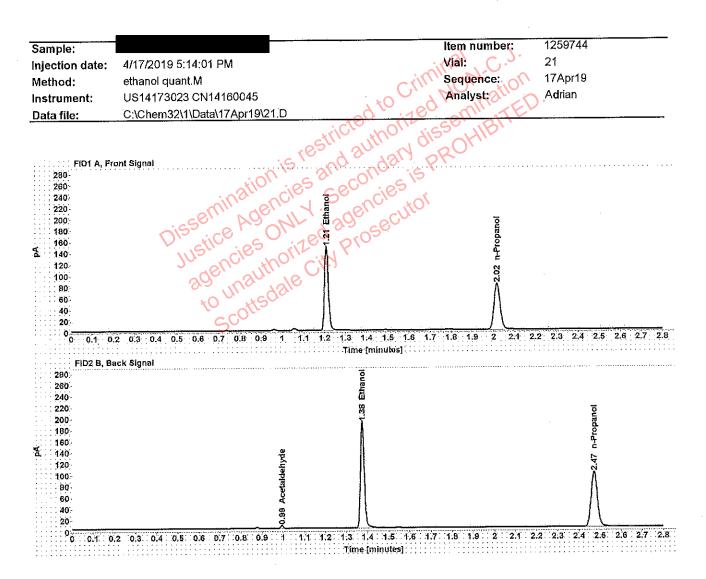


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,3040	1.209	189.151
n-Propanol		2.016	163,361


#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.791
Ethanol	1,375	235,283
n-Propanol	2.472	199,568

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

## Case:

## Scottsdale Police Department Crime Lab Volatiles Analysis

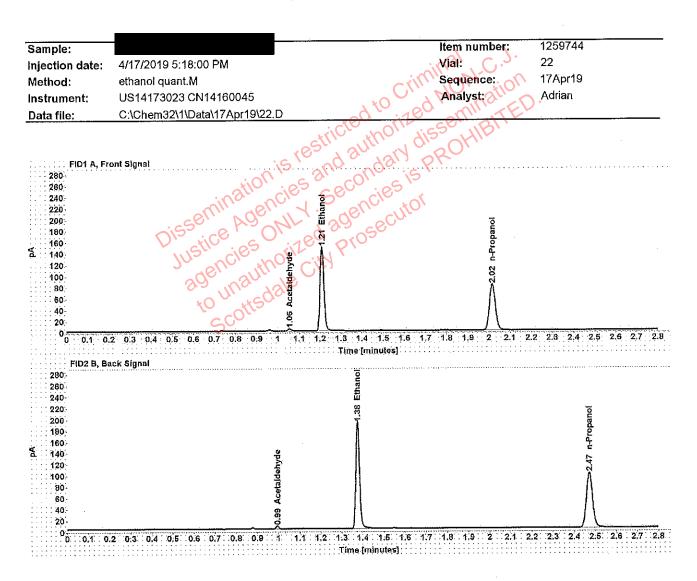

#### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	3.796
>Ethanol	0.3042	1.209	189.933
n-Propanol		2.016	163.938

Compound	Time (min)	Peak Area
Acetaldehyde	0,994	4.972
Ethanol	1.375	236,759
n-Propanol	2,471	200.361

# : Adrian, William - (18-Apr-2019)

Jser: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

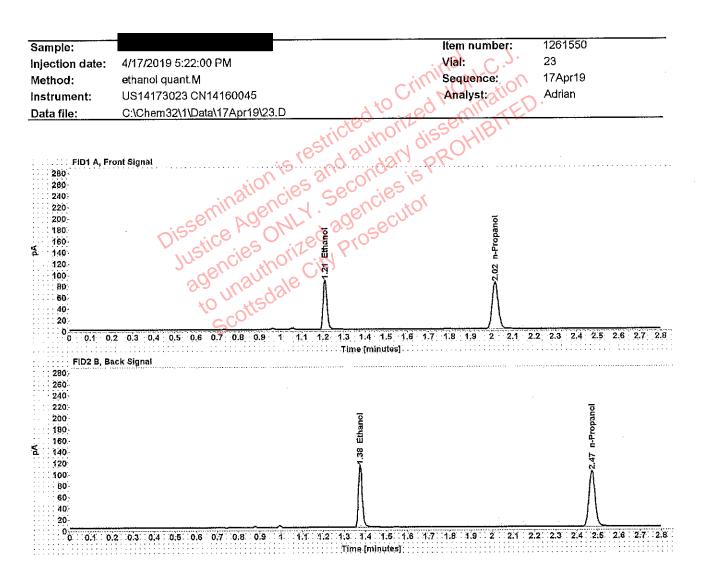

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1774	1.209	111.770
n-Propanol		2.016	166.044

#### Table 2: FID 2 B (column DB-ALC2)


Compound	Time (min)	Peak Area
Ethanol	1.375	138,436
n-Propanol	2.471	203,107

Case

### Adrian, William - (18-Apr-2019) Jser: wadrian 4/18/2019

### Case:

## Scottsdale Police Department Crime Lab Volatiles Analysis

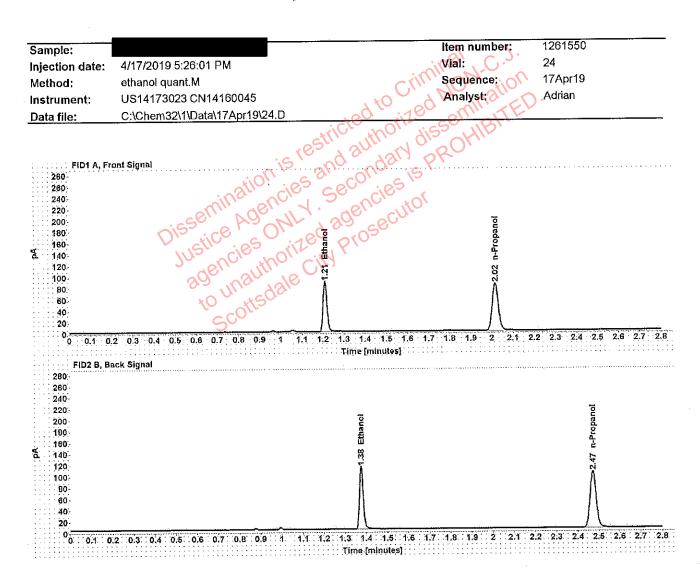


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1770	1.210	112.635
n-Propanol		2.016	167.736

Compound	Time (min)	Peak Area
Ethanol	1.376	140.234
n-Propanol	2.472	205.043

User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

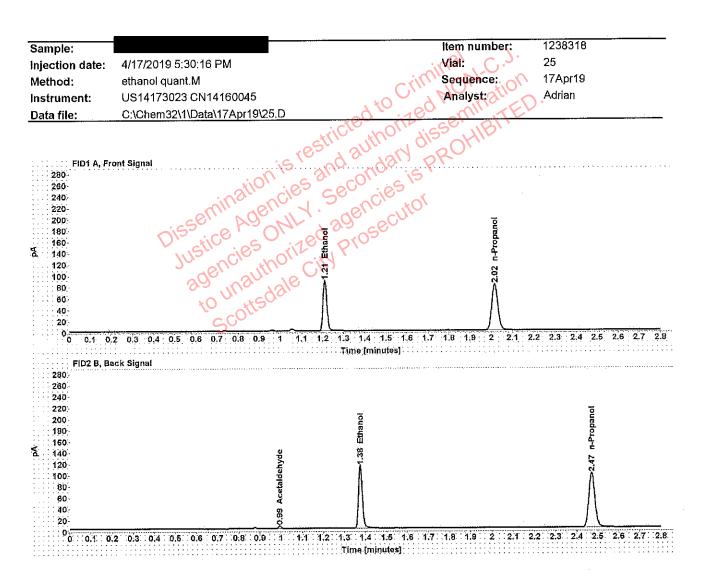

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1839	1.209	113.144
n-Propanol		2.016	162.051

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,994	4.515
Ethanol	1,375	140.621
n-Propanol	2,471	198,252

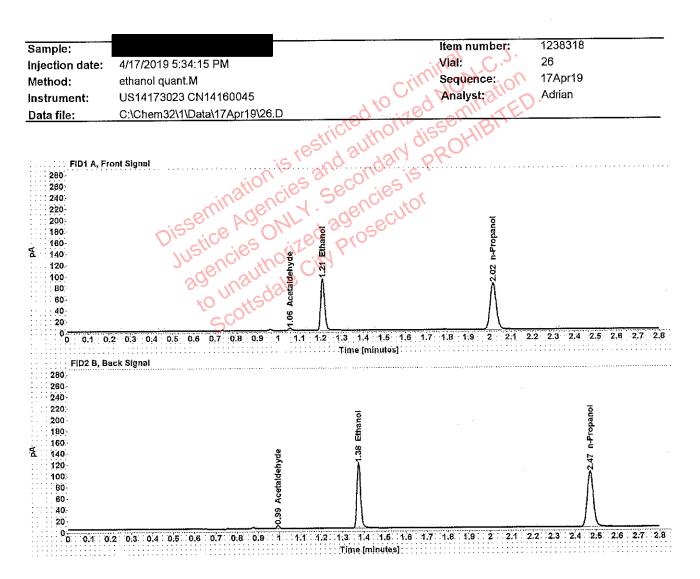


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.222
>Ethanol	0,1859	1.209	116,797
n-Propanol		2.016	165.510

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	5.540
Ethanol	1,375	144.754
n-Propanol	2.471	202.056

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

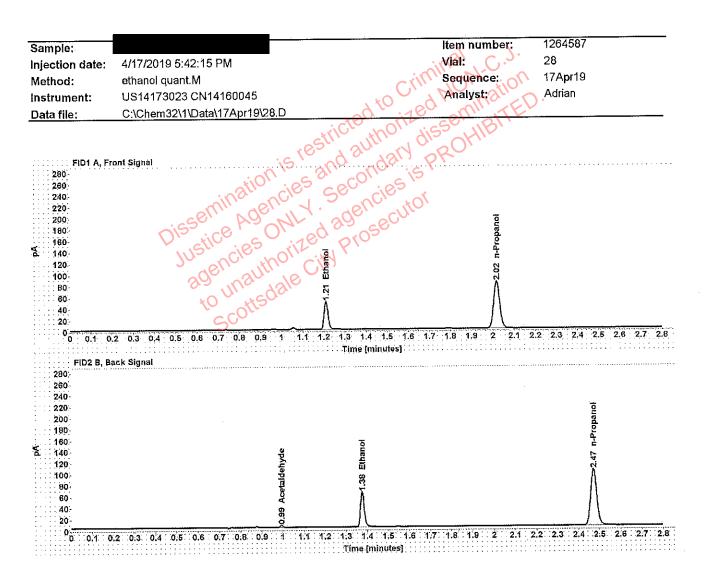


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1002	1.210	63,183
n-Propanol		2.016	167.243

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,993	3.897
Ethanol	1.376	78,069
n-Propanol	2.471	204.371

User: wadrian 4/18/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

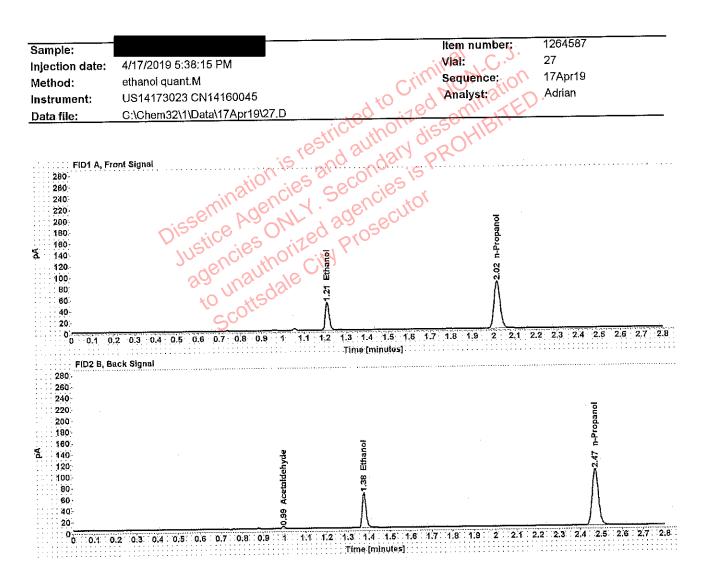


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanoi	0.1003	1.210	63.551
n-Propanol		2,016	168.045

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	3.956
Ethanol	1,376	78.534
n-Propanol	2.472	205.400

Jser: wadrian 4/18/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

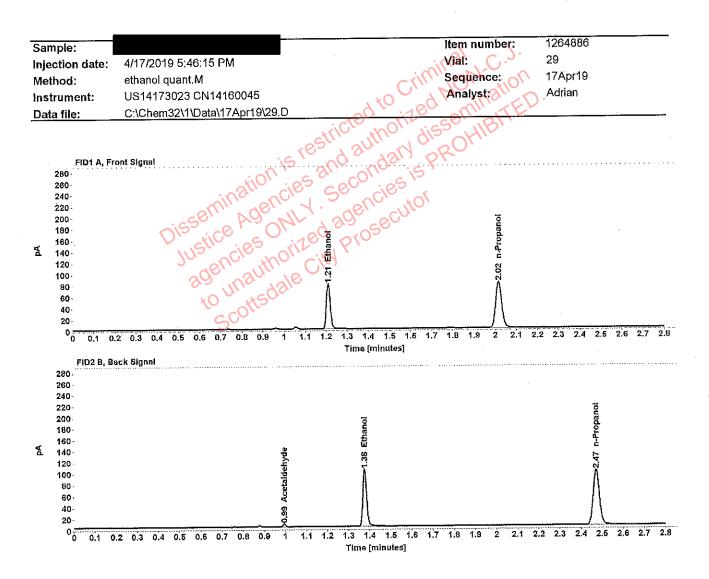


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1651	1,210	102.147
n-Propanol		2.016	163.170

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.711
Ethanol	1,376	127.140
n-Propanol	2.471	199.427

User: wadrian 4/18/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

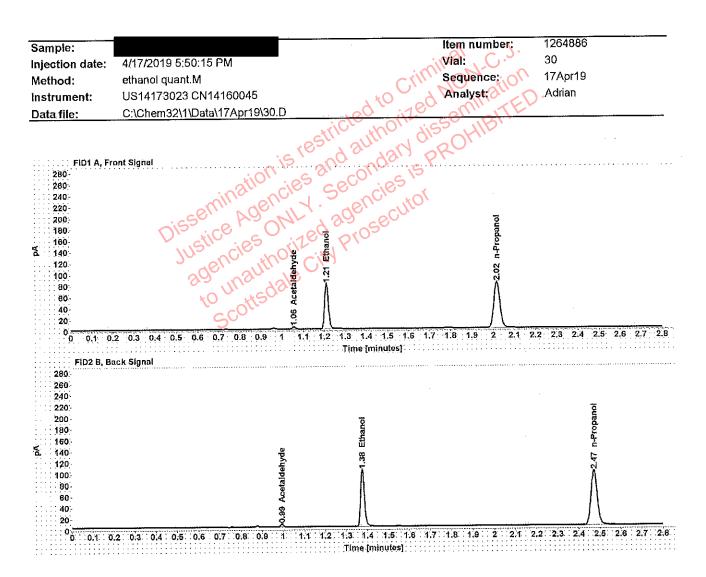


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	3.871
>Ethanol	0.1655	1.210	102.427
n-Propanol		2.016	163,151

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5.085
Ethanol	1.376	127.607
n-Propanol	2.472	199.355

User: wadrian 4/18/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis

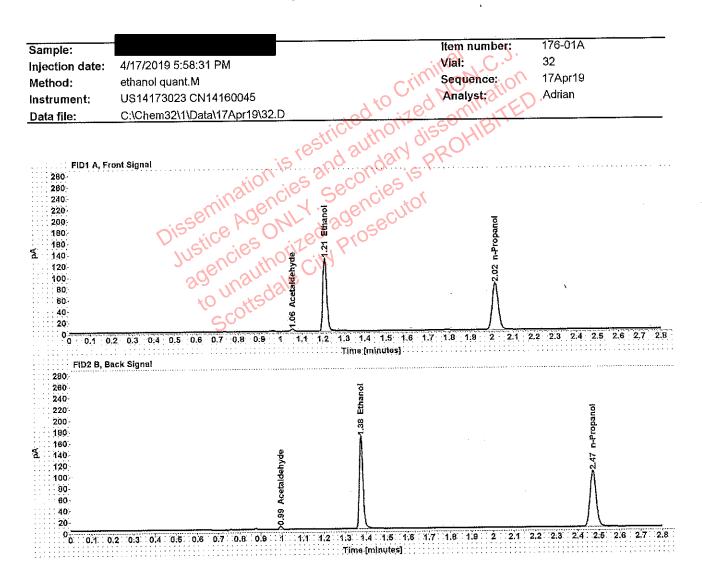

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.119
>Ethanol	0.2605	1.209	165.503
n-Propanol		2.016	166.990

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5.418
Ethanol	1.375	205.954
n-Propanol	2.472	203,686

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

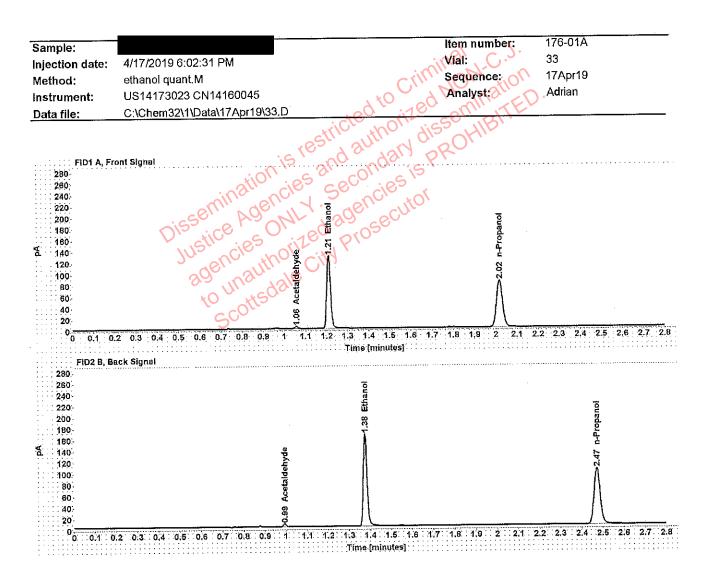


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area	
Acetaldehyde		1.055	3.836	
>Ethanol	0.2593	1,209	164.515	
n-Propanol		2.016	166.717	

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5.054
Ethanol	1,376	205.426
n-Propanol	2.472	203.746

Jser: wadrian 4/18/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis


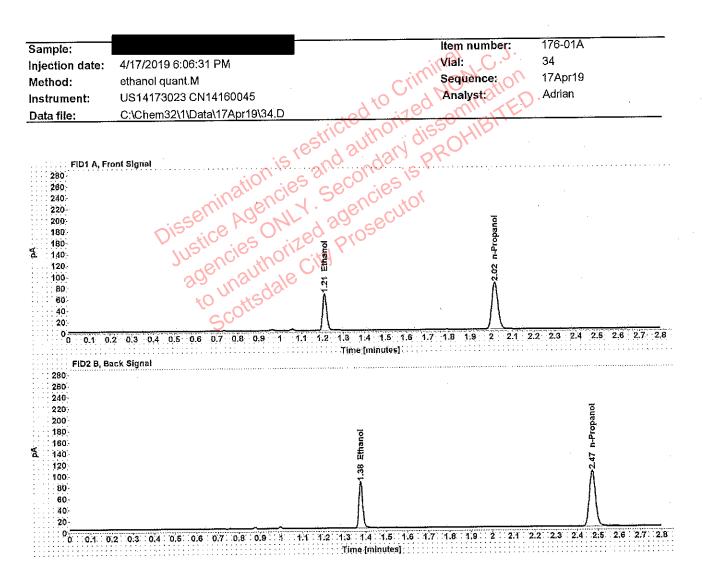


Table 1: FID 1 A (column DB
-----------------------------

Compound	Amount (g/100mL)	Time (min)	Peak Area	
>Ethanol	0.1328	1.210	83,829	
n-Propanol		2.016	166.833	

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.376	103.501
n-Propanol	2.472	203,257

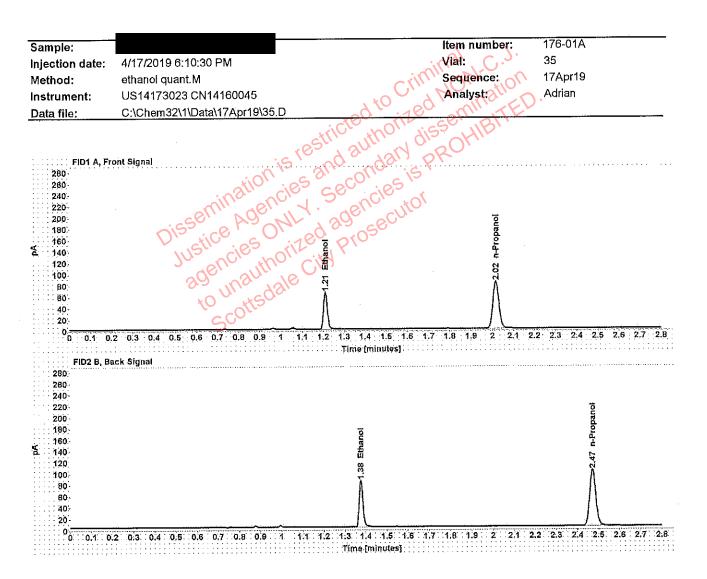

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area	
>Ethanol	0.1322	1.210	83,416	
n-Propanol		2,016	166.768	

Compound	Time (min)	Peak Area
Ethanol	1.376	103.218
n-Propanol	2,471	203.179

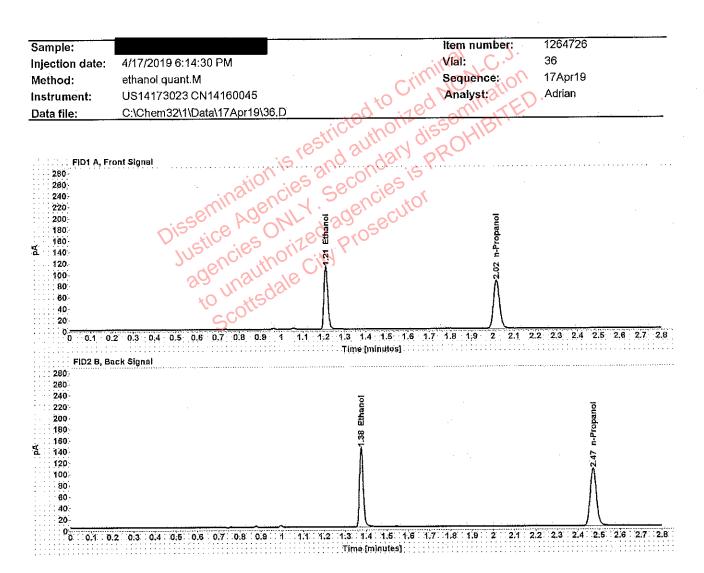


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2191	1.210	141.401
n-Propanol		2,017	169.781

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.376	176.008
n-Propanol	2,472	208,884

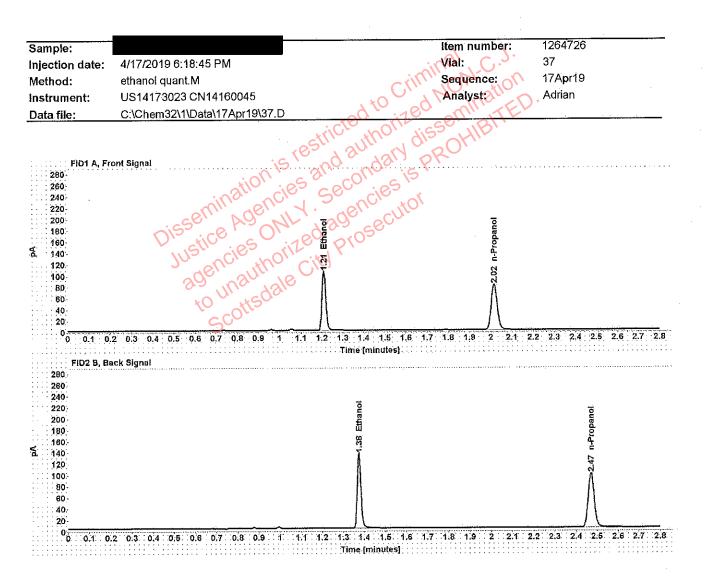


Table 1:	FID 1	A (column	DB-ALC1)
----------	-------	-----------	----------


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2184	1.209	133.911
n-Propanol		2,016	161.284

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.375	166.717
n-Propanol	2.471	198.242

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

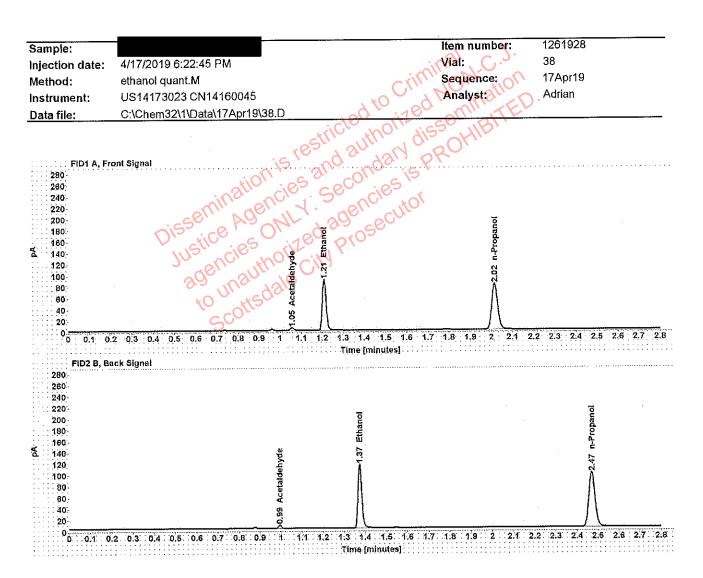

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.715
>Ethanol	0.1856	1.209	114.541
n-Propanol		2.016	162.594


### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,992	6.136
Ethanol	1.375	142.879
n-Propanol	2.471	198.991

### : Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

Case:

# Scottsdale Police Department Crime Lab Volatiles Analysis

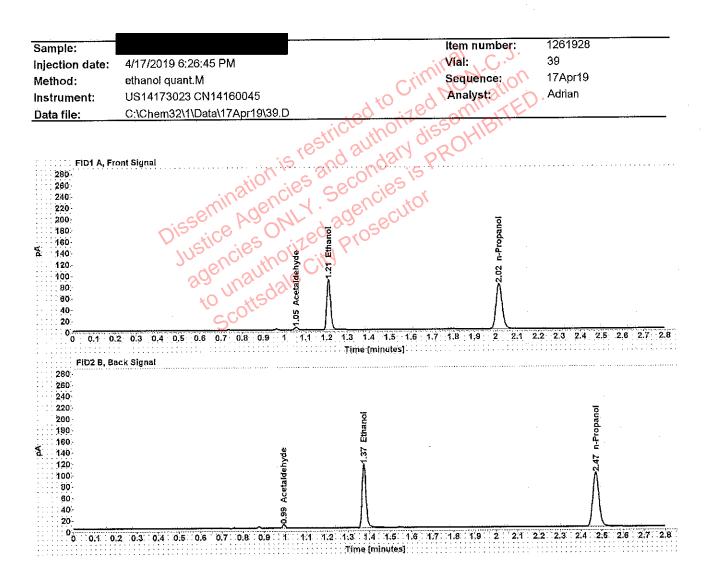


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.857
>Ethanol	0.1865	1.209	113.733
n-Propanol		2.016	160,670

Compound	Time (min)	Peak Area
Acetaldehyde	0.992	6.328
Ethanol	1,375	141.764
n-Propanol	2.471	196.444

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

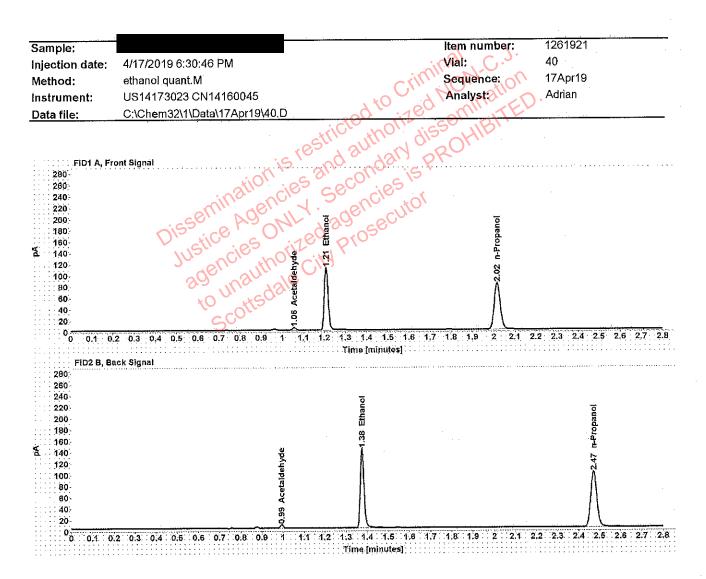

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.713
>Ethanol	0.2252	1.209	141.518
n-Propanol		2.016	165.300

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	6,183
Ethanol	1.375	176.170
n-Propanol	2.471	202.316

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

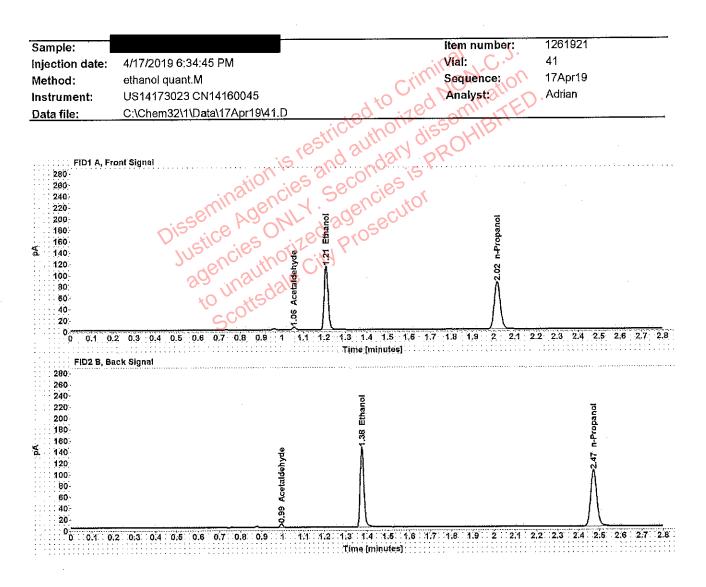


Table 1: FID 1	A (column	DB-ALC1)
----------------	-----------	----------


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.668
>Ethanol	0.2257	1.209	143.352
n-Propanol		2.016	167.100

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,994	6.140
Ethanol	1.375	178.291
n-Propanol	2.471	204.727

Jser: wadrian 4/18/2019

## Scottsdale Police Department Crime Lab Volatiles Analysis

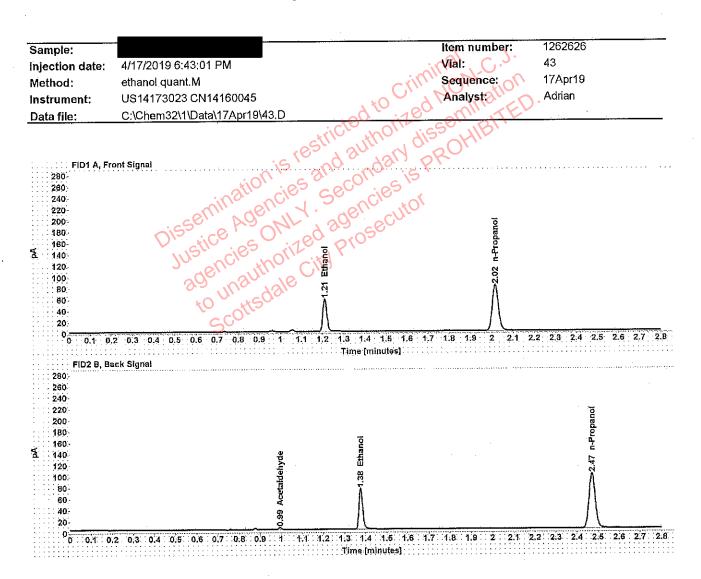


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1200	1,210	74.358
n-Propanol		2.016	163,929

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldenyde	0,994	3.796
Ethanol	1.376	91.819
n-Propanol	2.471	200.538

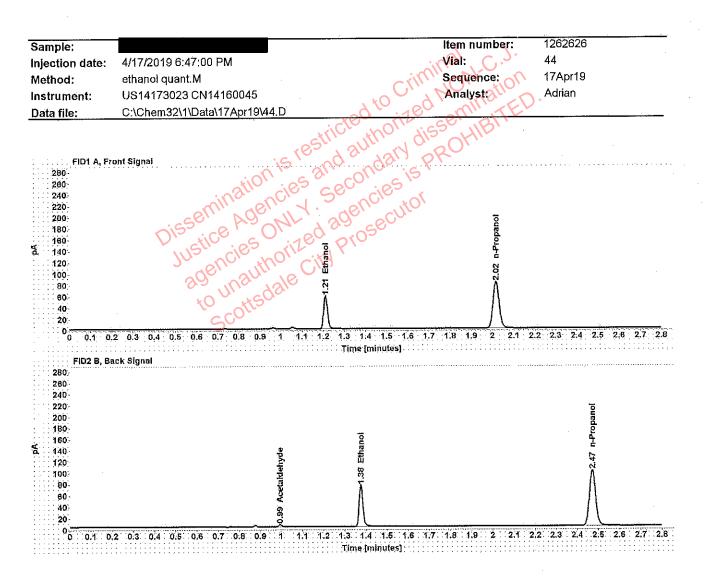

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1200	1.210	74.699
n-Propanol		2.016	164.672

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	3,809
Ethanol	1.376	92.598
n-Propanol	2.471	201.380

Jser: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

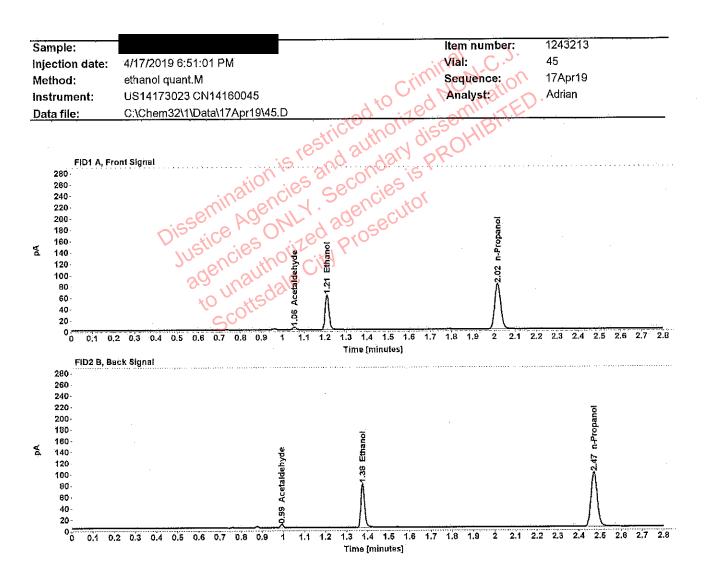


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.740
>Ethanol	0.1296	1.210	78.987
n-Propanol		2.016	161.113

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	6.190
Ethanol	1,375	97.587
n-Propanol	2.471	197.274

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

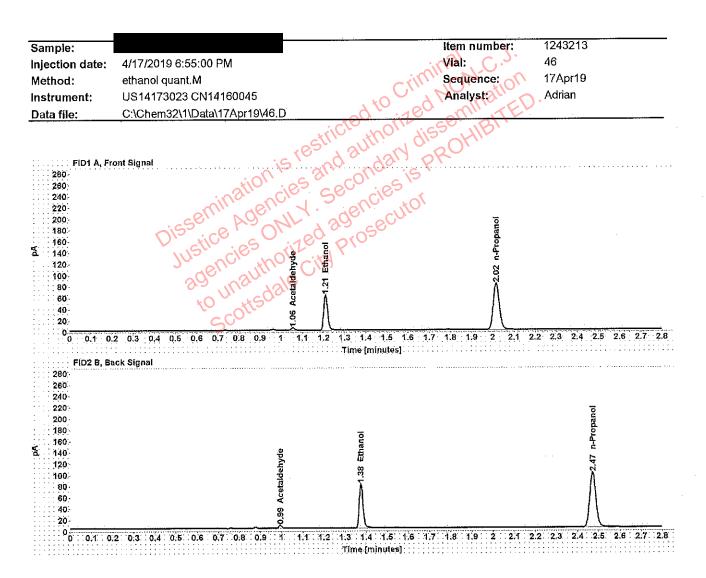


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4.318
>Ethanol	0.1286	1,210	79.533
n-Propanol		2.016	163.483

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,993	5.664
Ethanol	1.375	98.561
n-Propanol	2.471	200,092

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

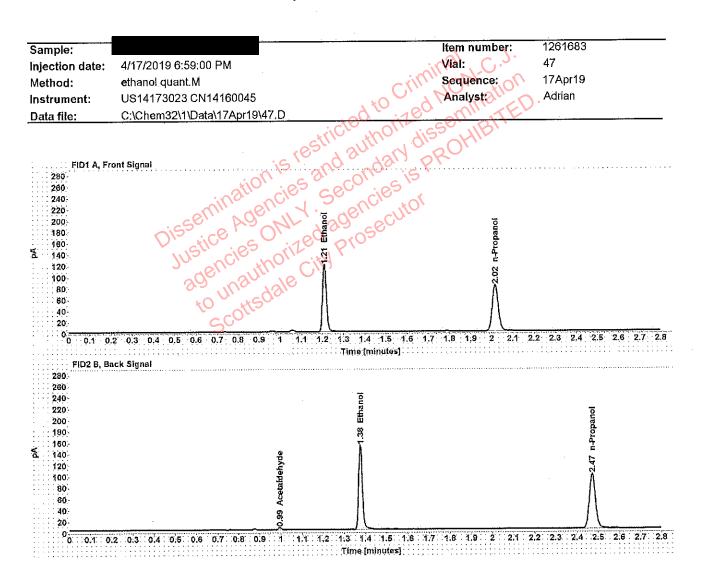


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2441	1.209	151,923
n-Propanol		2.016	163.607


### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.049
Ethanol	1,376	189.155
n-Propanol	2.471	199.790

### : Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

Case:

## Scottsdale Police Department Crime Lab Volatiles Analysis

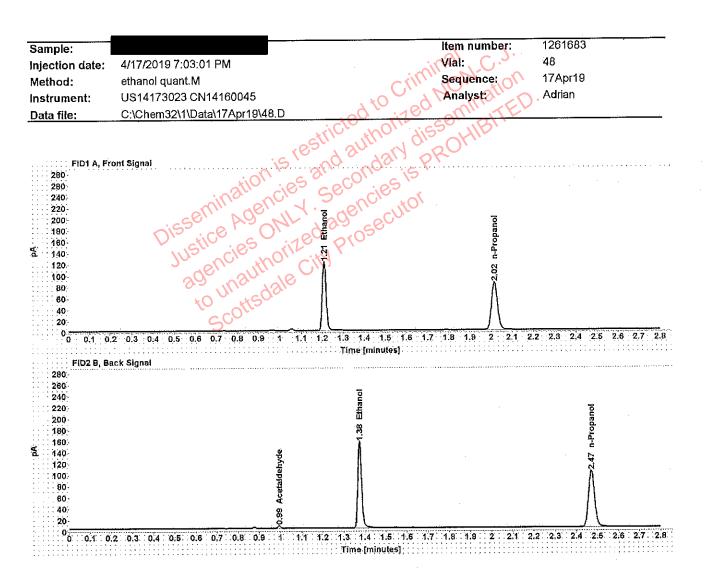


#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2419	1.209	154.233
n-Propanol		2.016	167.622

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.198
Ethanol	1,375	192.295
n-Propanol	2.471	205.533

Jser: wadrian 4/18/2019


### Scottsdale Police Department Crime Lab Volatiles Analysis

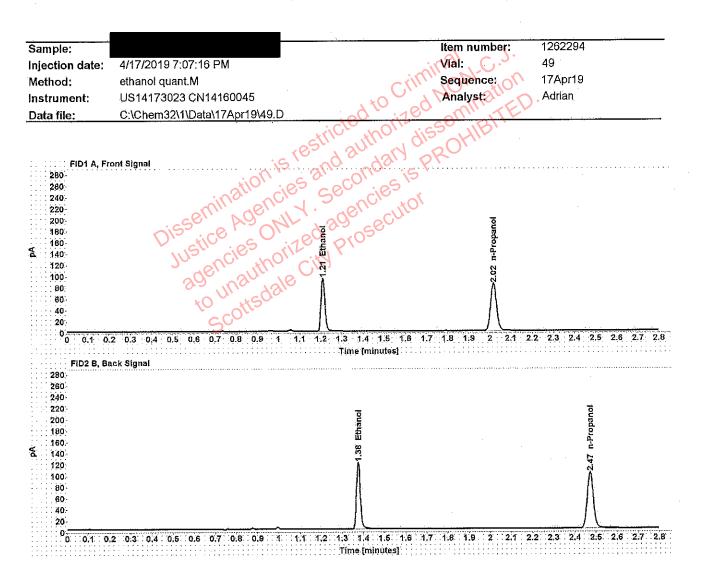

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1891	1.210	119.850
n-Propanol		2.016	166.952

Compound	Time (min)	Peak Area
Ethanol	1.376	148.925
n-Propanol	2.472	204.406

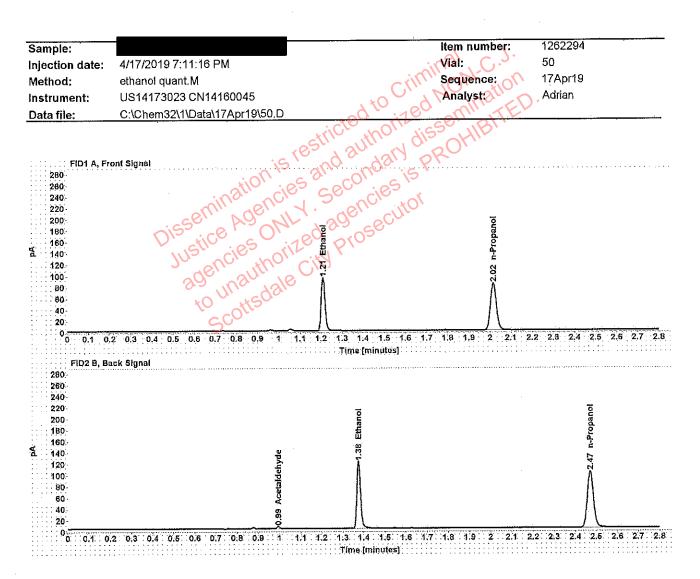

#### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1897	1.209	120.214
n-Propanol	*****	2.016	166.904

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,994	3.850
Ethanol	1.375	149.820
n-Propanol	2.471	204,365

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

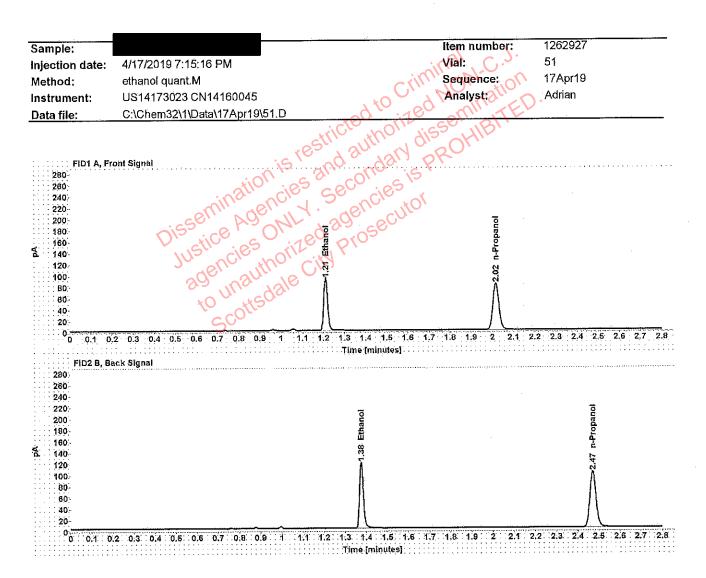


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0,1888	1.210	118.722
n-Propanol		2.016	165.642

Compound	Time (min)	Peak Area
Ethanol	1.376	147.723
n-Propanol	2,472	203.061

### : Adrian, William - (18-Apr-2019) Jser: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

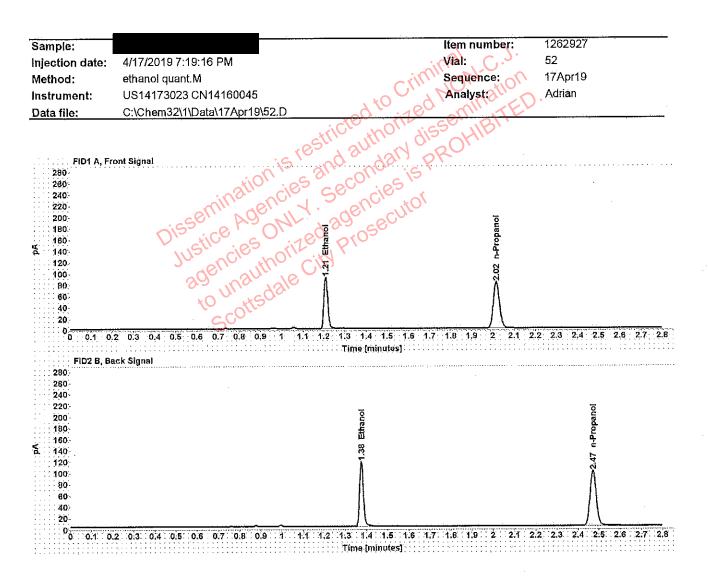

#### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1869	1.209	116,279
n-Propanol		2.016	163.855

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.376	144.862
n-Propanol	2.471	200.309

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

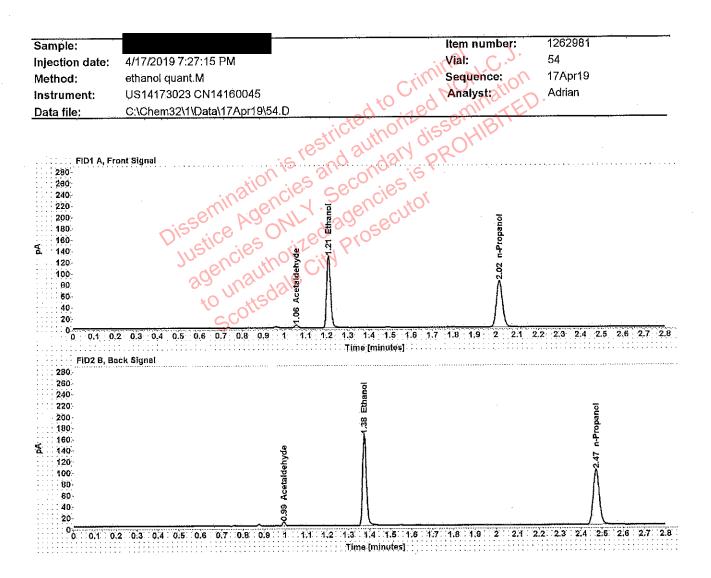

#### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	5.099
>Ethanol	0.2605	1,209	162.574
n-Propanol		2.016	164.029

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	6.687
Ethanol	1.375	202.328
n-Propanol	2.472	200.818

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

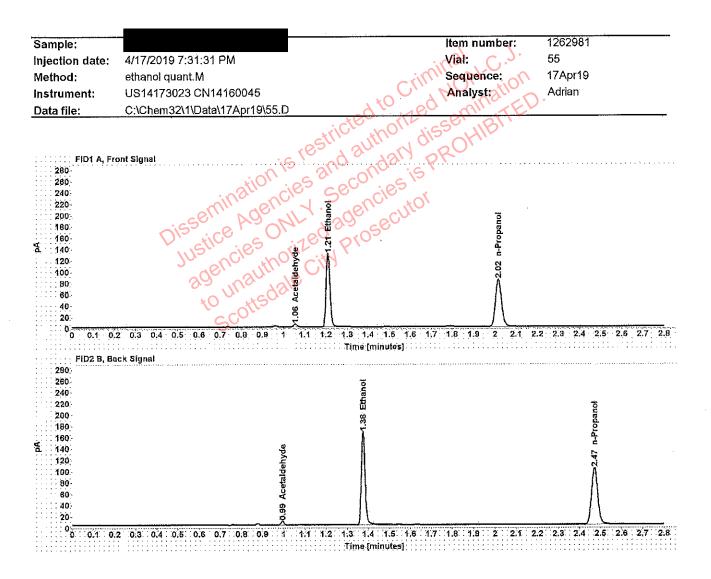

#### Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	5.127
>Ethanol	0.2607	1.209	165.889
n-Propanol		2.016	167.248

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	6,745
Ethanol	1.375	206.786
n-Propanol	2.472	204.599

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

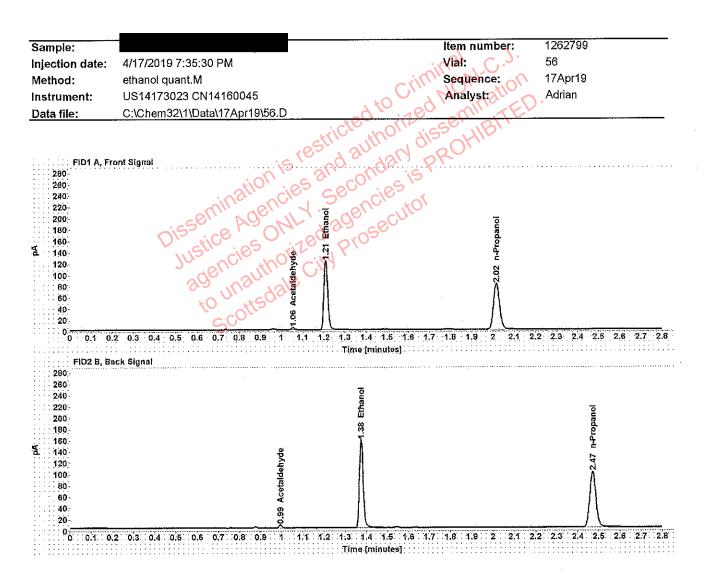

### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	3.955
>Ethanol	0,2506	1,209	156.502
n-Propanol		2.016	164.146

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5.186
Ethanol	1,375	195.071
n-Propanol	2.471	201.493

### : Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

# Scottsdale Police Department Crime Lab Volatiles Analysis


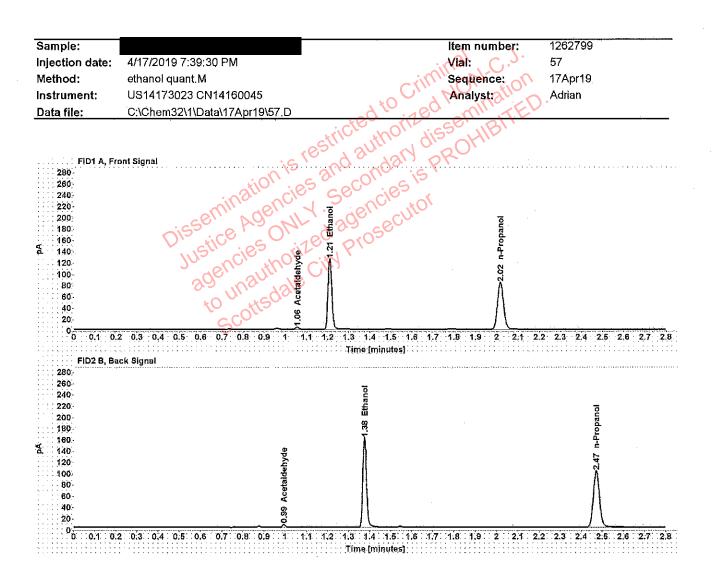


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	3.959
>Ethanol	0,2522	1.209	159,951
n-Propanol		2.016	166.728

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	5.218
Ethanol	1.376	199.319
n-Propanol	2.472	204.566

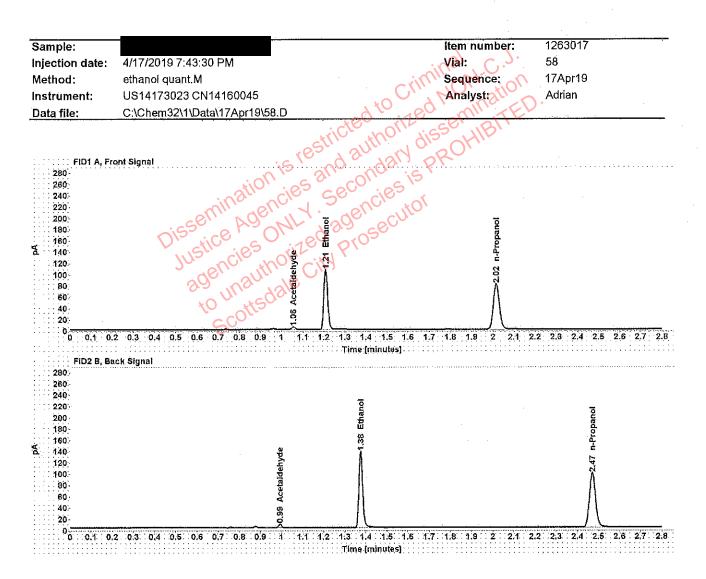

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	4,541
>Ethanol	0.2224	1,209	135.938
n-Propanol		2.016	160.773

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0,993	5.965
Ethanol	1.375	169.153
n-Propanol	2.471	196.781

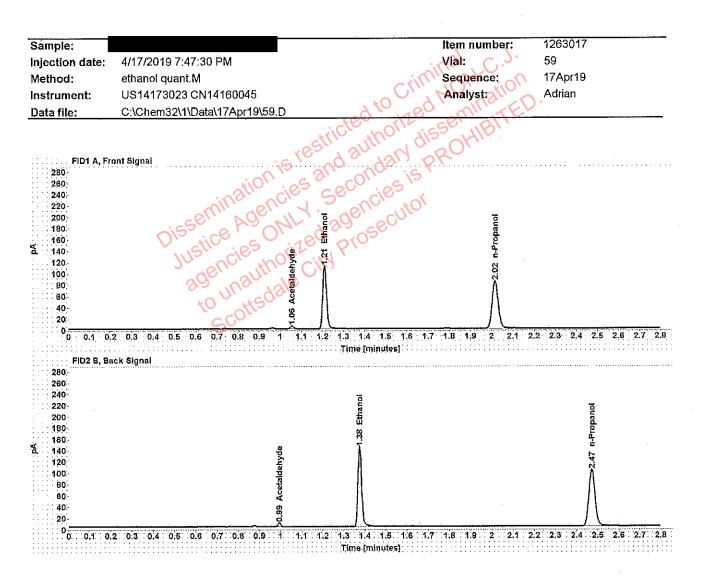


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
Acetaldehyde		1.055	5.119
>Ethanol	0.2232	1,209	141,893
n-Propanol		2.016	167.253

### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	6,699
Ethanol	1.375	177.244
n-Propanol	2.471	205,195

User: wadrian 4/18/2019

### Scottsdale Police Department Crime Lab Volatiles Analysis

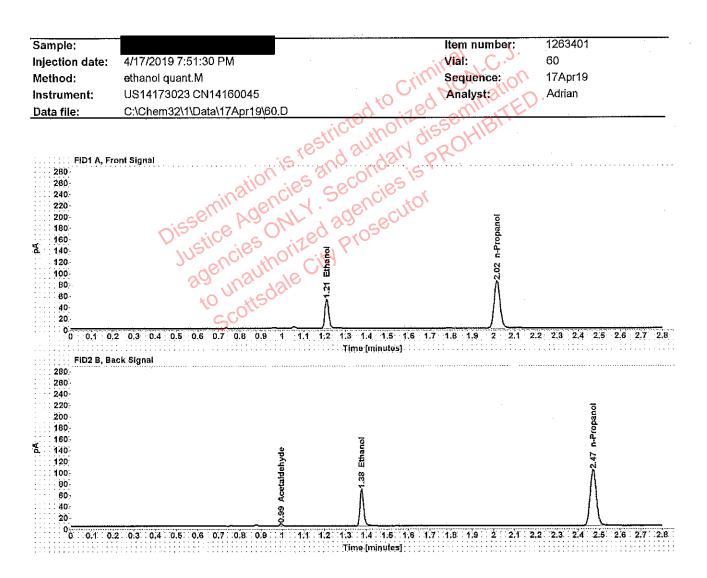

#### Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (mìn)	Peak Area
>Ethanol	0,1051	1.210	66.116
n-Propanol		2.016	166.702

#### Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.994	4.044
Ethanol	1.376	81.785
n-Propanol	2.471	203.551

### Adrian, William - (18-Apr-2019) User: wadrian 4/18/2019

Case:

Scottsdale Police Department Crime Lab Volatiles Analysis

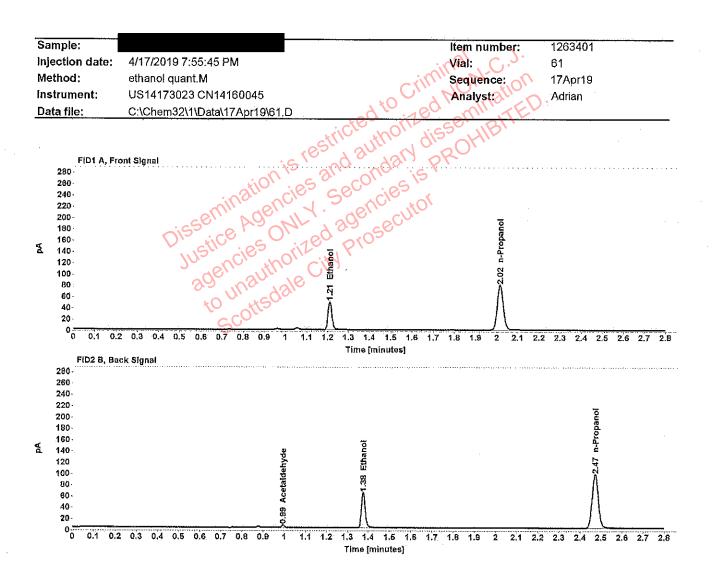


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1056	1.210	63.912
n-Propanol		2.016	160,433

Compound	Time (min)	Peak Area
Acetaldehyde	0.993	4.253
Ethanol	1.376	78.979
n-Propanol	2.471	195.769