SCOTTSDALE POLICE DEPARTMENT CRIME LABORATORY BLOOD ALCOHOL FACE SHEET

ANALYSIS DATE _	2/22/23	SEQUENCE NAM	ME <u>22Feb23</u>		
EQUIPMENT Pipettor Gas Chromatograph	Hamilton ML600EH	7497 Hamilton	ML600GJ10749		
INSTRUMENT CALIB	PATION	thorized Hamilion, who have disserted to the control of the contro	BITEL		
	restitution of the state of the	Utilian dis Oki			
Vial 1 0.02 calibrator Lot	FN10051909	Coeff	ficient of determination (r ²)		
Vial 2 0.10 calibrator Lot	FN05311902	105 S	0.99996		
Vial 3 0.20 calibrator Lo	FN02052101	ncies is ProCoeff			
Vial 4 0.40 calibrator Lo	FN03052102	0560			
IUSTIC	cies north th				
CALIBRATION VERI	EICATION AND RE	SOLUTION TEST			
0	7, " COO.	,			
Vial Sample	Expected result	Measured result	Manufacturer/lot		
5 Blank	Not detected	Not detected	SPD lab 122022AQ		
6 Volatiles mix	6 compounds	6 compounds	SPD lab 050721MIX		
7 Aqueous control	0.400 g/dL	0.399 g/dL	Lipomed 30012020-A		
8 Aqueous control	0.040 g/dL	0.040 g/dL	Lipomed 14082019-B		
9 Blood control	0.199 g/dL	0.205 g/dL	ACQ 4110320133/10		
20 Aqueous control	0.080 g/dL	0.080 g/dL	Lipomed 20012020-B		
31 Blood control	0.199 g/dL	0.205 g/dL	ACQ 4110320133/10		
42 Aqueous control	0.080 g/dL	0.079 g/dL	Lipomed 20012020-B		
49 Aqueous control	0.400 g/dL	0.402 g/dL	Lipomed 30012020-A		
50 Aqueous control		0.040 g/dL	Lipomed 14082019-B		
51 Blood control	0.199 g/dL	0.206 g/dL	ACQ 4110320133/10		
52 Blank	Not detected	Not detected	SPD lab 011823WB		
<u> </u>		· · · · · · · · · · · · · · · · · · ·	<u>and the second </u>		
<u> </u>		·.			
SUBJECT SAMPLES					
Subjects in the sequence	14 Sub	jects requiring reanaly	/sis0		
ADDITIONAL NOTES: All		was atod. The was also	included four proficional		
ADDITIONAL NOTES: All samples. Item 402-1R.E. (I					
hand corrected on all supp		miliany listed incorrect	ly as 402-2R.E. but was		
nand corrected on an supp	orting documentation.				
Run valid 🛛 🏏	K	Run valid 🛛	· 1/ / ·		
Run invalid 🗌 U he	De Brook	Run invalid 🔲 🔃 🗘	Wa Camonico		
Ar	alyst		Technical Reviewer		

Document ID: 1208 Revision Date:02/27/2017 Issuing Authority: Kris Cano, Forensic Services Director

Page 1 of 1


Scottsdale Police Department Crime Laboratory Sequence Quality Assurance Summary

SEQUENCE NAME: 22Feb23

ANA	LYST	: Broo	ke
-----	------	--------	----

Sample Name	Vial	Measured Value (g/dL)	Expected Value (g/dL)	Percent Difference	Absolute Difference (g/dL)
blank 122022AQ	5	negative	negative	-100	د.0٠
0.400 30012020-A	7	0.399	0.400	0.25	-0.001
0.040 14082019-B	8	0.040	0.040	S 0.00	0.000
0.199 4110320133/10	- 9	0.205	0.199	3.02	0.006
0.080 20012020-B	20	0.080	0.080	0.00	0.000
0.199 4110320133/10	31	0.205	0.199	3.02	0.006
0.080 20012020-B	42	0.079	0.080	1.25	-0.001
0.400 30012020-A	49	0.402	0.400	0.50	0.002
0.040 14082019-B	50	0.040	0.040	0.00	0.000
0.199 4110320133/10	51	0.206	0.199	3.52	0.007
blank 011823WB	52	S negative	negative	_	-

Calibrator	Ethanol Area	N-propanol Area	Ratio
0.020	11.862	163.294	0.073
0.100	59.785	162.479	0.368
0.200	121.962	162.456	0.751
0.400	240,421	161.112	1,492

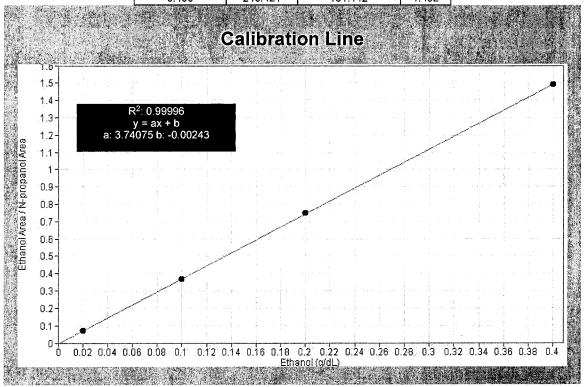

Sample: Description: FN10051909

0.020 calibrator

Method:

ethanol quant.M

Instrument:

US14173023 CN14160045

Data file:

Vial:

Sequence:


22Feb23

Injection date:

2/22/2023 12:02:26 PM

Analyst: Brooke

C:\Chem32\1\Data\22Feb23\1.D

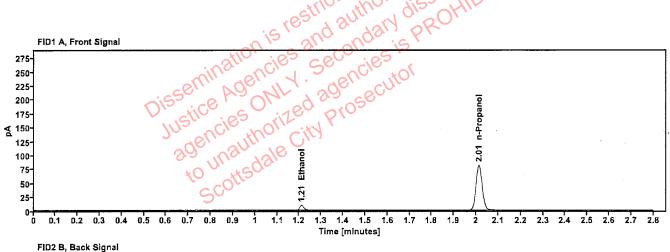

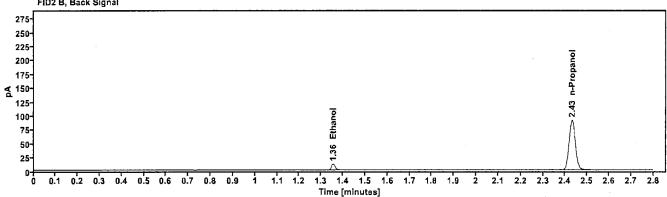


Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.210	11.862
n-Propanol	2.013	163.294

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.355	12.856
n-Propanol	2.432	177.845

Sample: Description: FN05311902

0.100 calibrator

Vial: Sequence:

22Feb23

2

Method:

ethanol quant.M

Injection date:

2/22/2023 12:06:26 PM


Instrument:

US14173023 CN14160045

Analyst: Bro

Brooke $\sqrt{}$

Data file: C:\Chem32\1\Data\22Feb23\2.D

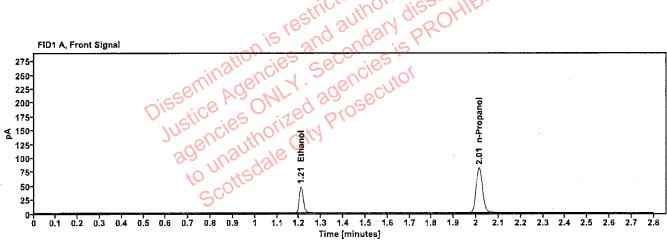

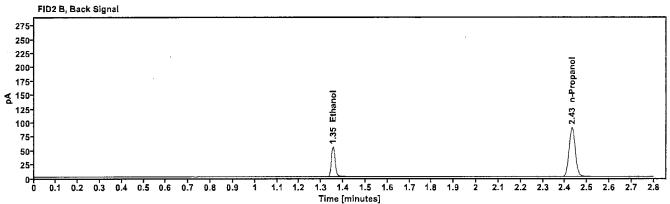


Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.208	59.785
n-Propanol	2.013	162.479

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.354	65.357
n-Propanol	2.432	176.840

Sample:

FN02052101

Description:

0.200 calibrator

Method:

ethanol quant.M

Instrument: Data file:

US14173023 CN14160045

C:\Chem32\1\Data\22Feb23\3.D

Vial:

Sequence:

Analyst:

Injection date:


22Feb23 2/22/2023 12:10:25 PM

Brooke

3

PB



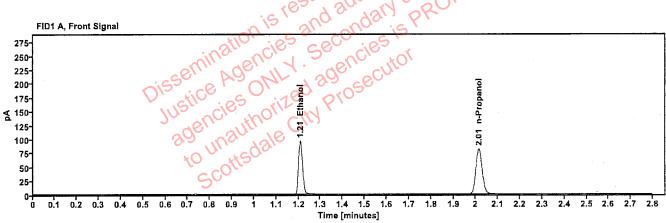

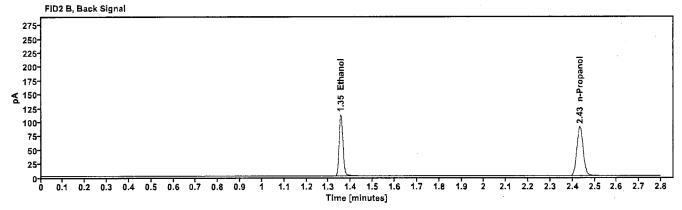


Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.208	121.962
n-Propanol	2.014	162.456

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.355	133,628
n-Propanol	2.433	176.692

Sample: FN03052102

Description: 0.400 calibrator

Method:

ethanol quant.M

Instrument: Data file: US14173023 CN14160045

C:\Chem32\1\Data\22Feb23\4.D

Vial:

Sequence:


22Feb23

Injection date:

2/22/2023 12:14:25 PM

Analyst: Brooke

ooke PB

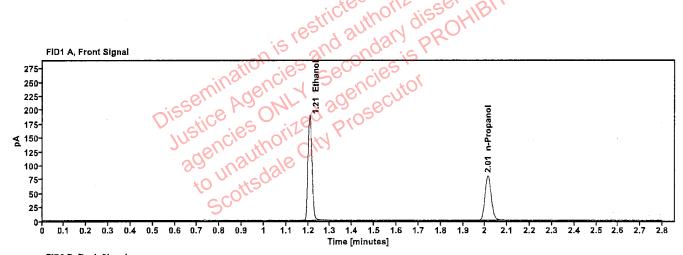

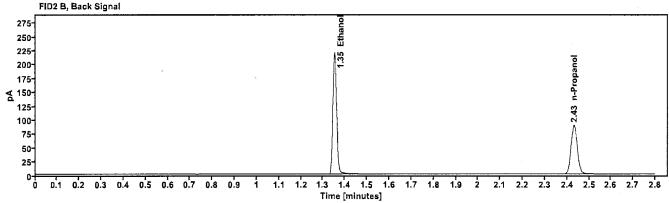



Table 1: FID 1 A (column DB-ALC1)

Compound	Time (min)	Peak Area
Ethanol	1.207	240.421
n-Propanol	2.013	161.112

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.353	264.492
n-Propanol	2.432	175.363

Sample: 122022AQ Vial: LIMS ID: **Description:** Negative Seguence: \. 22Feb23 Method: ethanol quant.M Injection date: 2/22/2023 12:18:26 PM Instrument: US14173023 CN14160045 Analyst: Brooke C:\Chem32\1\Data\22Feb23\5.D Data file:

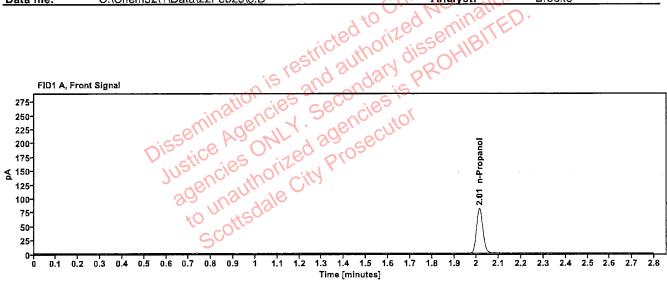

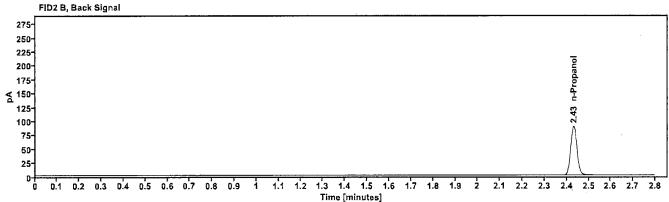


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.013	161.512

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.432	175.919


Sample: 050721MIX **Vial:** 6

Description: Volatiles mix LIMS ID:

 Method:
 ethanol quant.M
 Sequence:
 22Feb23

 Instrument:
 US14173023 CN14160045
 Injection date:
 2/22/2023 12:22:26 PM

Data file: C:\Chem32\1\Data\22Feb23\6.D Analyst: Brooke

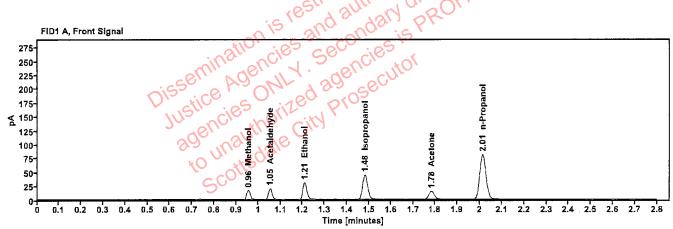

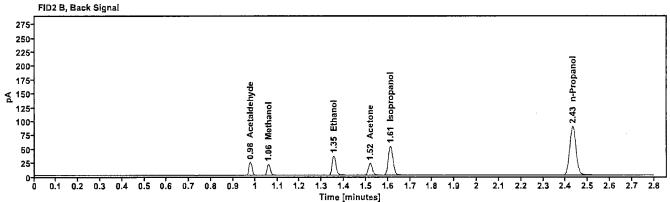


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
Methanol		0.956	18.898
Acetaldehyde		1.054	21.578
>Ethanol	0.0650	1.209	38.837
Isopropanol		1.482	70.839
Acetone		1.783	25.458
n-Propanol		2.014	161.458

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Acetaldehyde	0.978	24.190
Methanol	1.060	20.830
Ethanol	1.354	42.330
Acetone	1.519	27.977
Isopropanol	1.612	78.418
n-Propanol	2.432	175.666

Sample: 30012020-A Vial:


0.2 0.3 0.4 0.5 0.6 0.7 0.8 0.9 1 1.1 1.2 1.3 1.4 1.5 1.6 1.7 1.8 1.9

Description: 0.400 LIMS ID:

Method: ethanol quant.M Sequence: 22Feb23

Instrument: US14173023 CN14160045 Injection date: 2/22/2023 12:26:41 PN

Data file: C:\Chem32\1\Data\22Feb23\7.D Analyst: Brooke

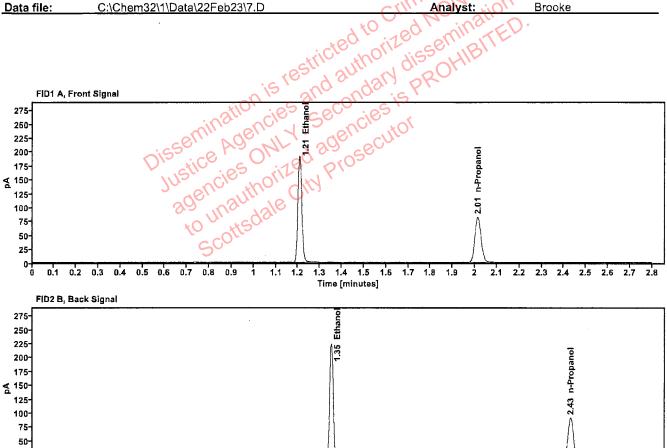

Time [minutes]

Table 1: FID 1 A (column DB-ALC1)

25-

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.3996	1.207	243.778
n-Propanol		2.014	163.345

Table 2: FID 2 B (column DB-ALC2)

2.3 2.4

2 2.1 2.2

Compound	Time (min)	Peak Area
Ethanol	1.354	268.010
n-Propanol	2.432	177.709

Sample: 14082019-B **Vial:** 8

Description: 0.040

Method: ethanol quant.M

Instrument: US14173023 CN14160045

Data file: C:\Chem32\1\Data\22Feb23\8.D


LIMS ID:

Sequence: \.

22Feb23

Injection date: 2/22/2023 12:30:41 PM

Analyst: Brooke

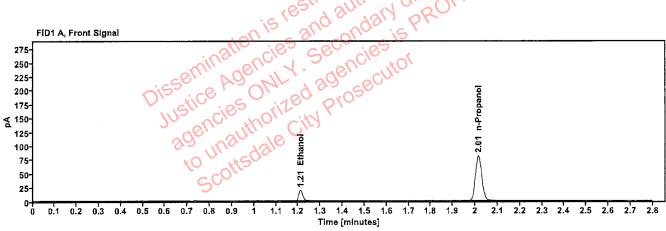

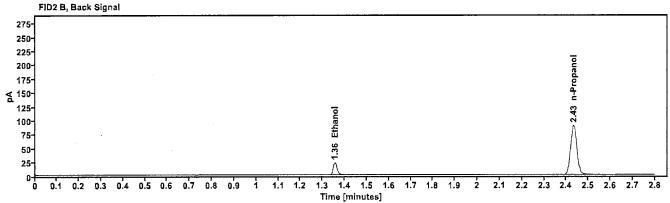


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0409	1.210	24.412
n-Propanol		2.014	162.232

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.356	26.576
n-Propanoi	2.433	176.472

Sample: Description:

4110320133/10

0.199

ethanol quant.M

Instrument:

Method:

US14173023 CN14160045

Data file: C:\Chem32\1\Data\22Feb23\9.D Vial:

LIMS ID:

Sequence: \


Injection date:

22Feb23

9

2/22/2023 12:34:40 PM

Brooke

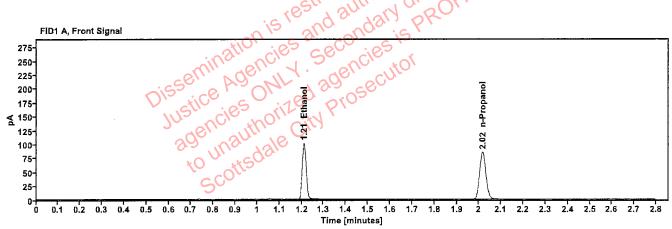

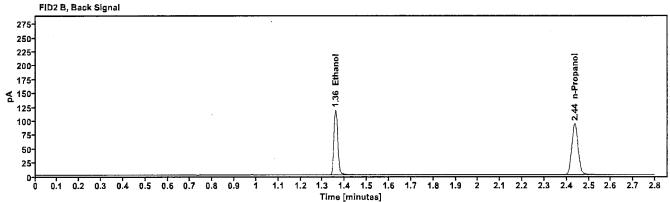


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2058	1.211	129.961
n-Propanol		2.016	169.367

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	142.729
n-Propanol	2.437	184.313

Sample: 20012020-B Vial: 20

Description: Method:

0.080

ethanol quant.M

Instrument:

US14173023 CN14160045

C:\Chem32\1\Data\22Feb23\20.D Data file:


LIMS ID:

Sequence: \

22Feb23 Injection date:

2/22/2023 1:19:11 PM

PB

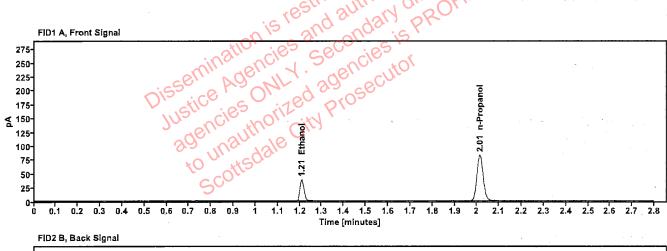

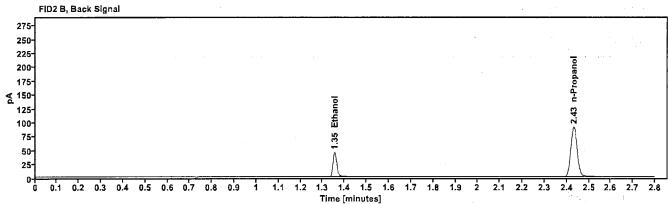


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0800	1.209	49.089
n-Propanol		2.014	165.333

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.355	53.612
n-Propanol	2.432	179.968

Sample: 4110320133/10 Vial:

Description: 0.199

Method: ethanol quant.M

Instrument: US14173023 CN14160045


Data file: C:\Chem32\1\Data\22Feb23\31.D 31

LIMS ID:

Sequence: \. 22Feb23

2/22/2023 2:03:40 PM Injection date:

Analyst: Brooke

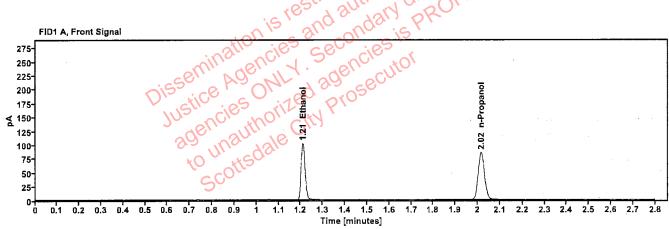

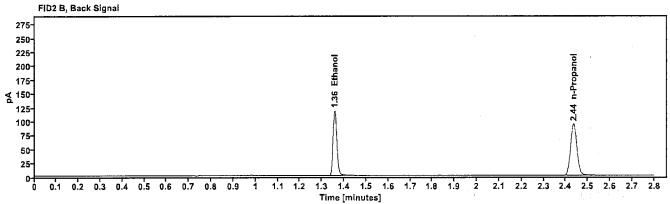


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2057	1.210	130.286
n-Propanol		2.016	169.863

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.358	142.183
n-Propanol	2.436	184.578

Vial: Sample: 20012020-B 42

Description: Method:

0.080

Instrument:

ethanol quant.M


US14173023 CN14160045

C:\Chem32\1\Data\22Feb23\42.D Data file:

LIMS ID:

Sequence: \ Injection date: 22Feb23

2/22/2023 2:47:57 PM

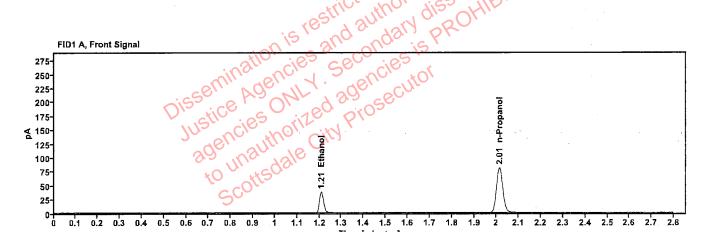

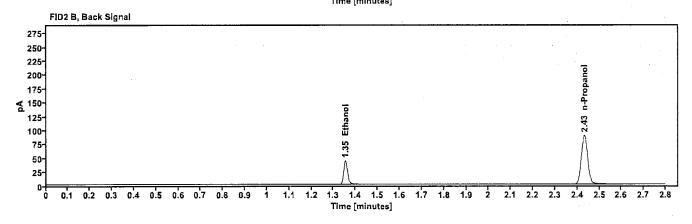


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0796	1.209	47.840
n-Propanol		2.013	162.063

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.354	52.317
n-Propanol	2.432	176.412

Sample: 30012020-A

Description:

Instrument:

Method:

0.400

ethanol quant.M US14173023 CN14160045

Data file: C:\Chem32\1\Data\22Feb23\49.D

Vial:

LIMS ID:

Sequence: \ Injection date:


22Feb23

49

2/22/2023 3:16:26 PM

alyst: Brooke

YB.

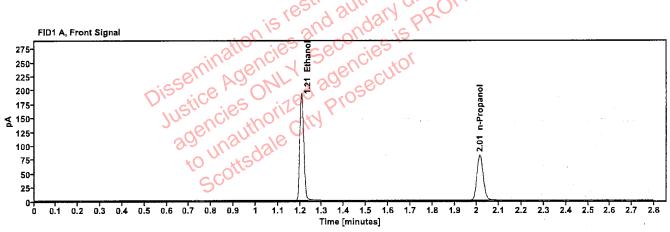

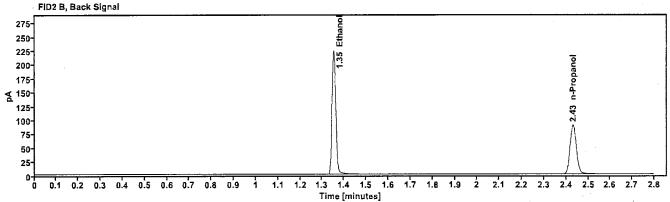


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.4020	1.207	244.687
n-Propanol		2.013	162.989

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.353	269.364
n-Propanol	2.432	177.232

Sample: Description: 14082019-B

0.040

Instrument:

Method:

ethanol quant.M

US14173023 CN14160045

Data file:

C:\Chem32\1\Data\22Feb23\50.D

Vial:


LIMS ID:

Sequence: \....

22Feb23 ...

Injection date: 2/22/2023 3:20:26 PM

50

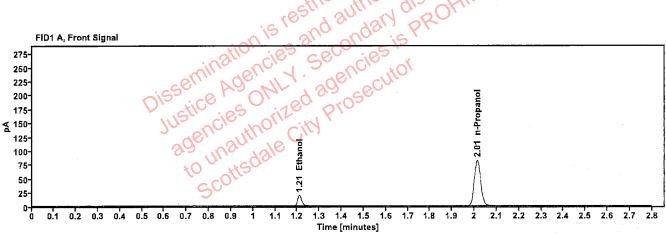

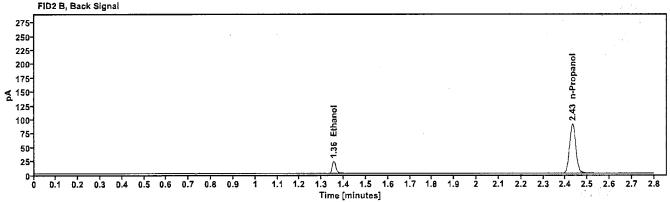


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0406	1.210	24.527
n-Propanol		2.014	164.034

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.355	26.860
n-Propanol	2.432	178.481

4110320133/10 Sample:

Description:

0.199

Method:

ethanol quant.M

Instrument: US14173023 CN14160045 Data file:

C:\Chem32\1\Data\22Feb23\51.D

Vial:

51


LIMS ID:

Sequence: \

Injection date:

22Feb23

2/22/2023 3:24:26 PM

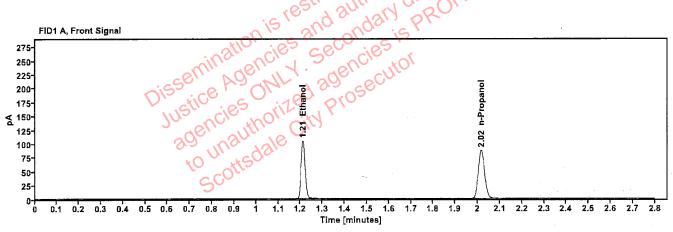

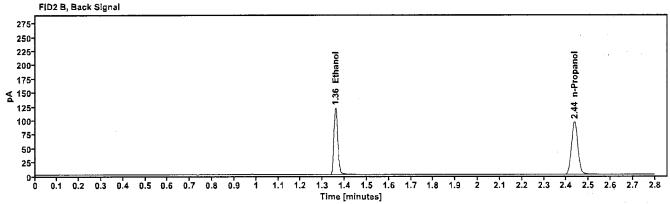


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2064	1.211	133.736
n-Propanol		2.016	173.738

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	146.876
n-Propanol	2.437	189.084

Sample: 011823WB **Vial:** 52

Description:

Negative

LIMS ID:

22Feb23

Method:

ethanol quant.M


Sequence: Injection date:

2/22/2023 3:28:26 PM

Instrument: Data file: US14173023 CN14160045

Data file: C:\Chem32\1\Data\22Feb23\52.D

Analyst: B

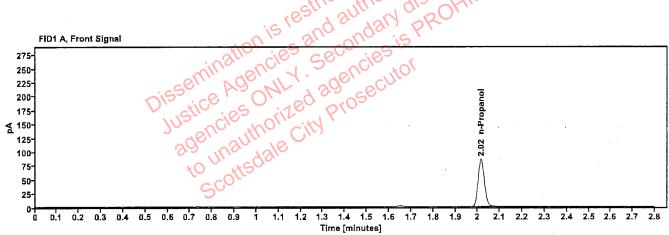

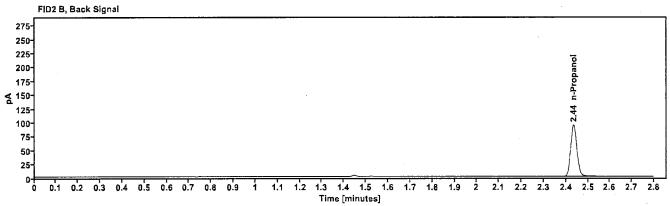


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.016	170.492

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.436	185.619

Sequence Summary

Page 1 of 2

Seque	nce name: 2	2Feb23 Instrument: U	S14173023 CN141600	45 Analys	st: Brooke
			· · · · · · · · · · · · · · · · · · ·	al	
Vial	Sample	Description	Type	LIMS ID	Method
1	FN10051909	0.020 calibrator	Calibration	Oh ation	ethanol quant.M
2	FN05311902	0.100 calibrator	Calibration	WILL ED.	ethanol quant.M
3	FN02052101	0.200 calibrator	Calibration C	31,1811	ethanol quant.M
4	FN03052102	0.400 calibrator	Calibration		ethanol quant.M
5	122022AQ	Negative (Control		ethanol quant.M
6	050721MIX	Volatiles mix	Control	***************************************	ethanol quant.M
7	30012020-A	0.400	Control	many or a related Miller Section with Lane to be an income of the	ethanol quant.M
. 8	14082019-B	0.040	Control		ethanol quant.M
9	4110320133/10	0.199	Control		ethanol quant.M
- 10	327-01A.B.)10 +1C8 -2 0 160	Sample		ethanol quant.M
11	327-01A.B.	W: No Colonia	Sample		ethanol quant.M
12		902-18.E	Sample		ethanol quant.M
13	-402-2R.E. 7-14-7	402-1 R.E	Sample		ethanol quant.M
14	420-01A.G.	to atte	Sample		ethanol quant.M
15	420-01A.G.	SCOT	Sample		ethanol quant.M
16	41902I.C.	demonent	Sample		ethanol quant.M
17	41902l.C. ,	Normania I	Sample		ethanol quant.M
18	423-01D.G.	general	Sample		ethanol quant.M
19	423-01D.G.	Queuen	Sample		ethanol quant.M
20	20012020-B	0.080	Control		ethanol quant.M
21	422-01A.W.		Sample		ethanol quant.M
22	422-01A.W.		Sample		ethanol quant.M
23	387-01E.C.		Sample		ethanol quant.M
24	387-01E.C.		Sample		ethanol quant.M
25	423-01V.W.		Sample		ethanol quant.M
26	423-01V.W.		Sample		ethanol quant.M
27	2303054-2		Sample		ethanol quant.M
28	2303054-2		Sample		ethanol quant.M
29	2303044-1		Sample		ethanol quant.M
30	2303044-1		Sample		ethanol quant.M
31	4110320133/10	0.199	Control		ethanol quant.M
32	2302949-1		Sample		ethanol quant.M
33	2302949-1		Sample		ethanol quant.M
34	2303151-4		Sample		ethanol quant.M
35	2303151-4		Sample		ethanol quant.M
36	2303161-2		Sample		ethanol quant.M
37	2303161-2		Sample		ethanol quant.M
38	2303142-2		Sample		ethanol quant.M
39	2303142-2		Sample		ethanol quant.M
40	VIAL00002		Sample		ethanol quant.M
41	VIAL00002		Sample		ethanol quant.M
42	20012020-B	0.080	Control		ethanol quant.M
43	VIAL00001		Sample		ethanol quant.M
44	VIAL00001		Sample		ethanol quant.M
45	VIAL00003		Sample		ethanol quant.M
46	VIAL00003		Sample		ethanol quant.M
47	VIAL00004		Sample		ethanol quant.M

B

PB

Sequence Summary

Page 2 of 2

	48	VIAL00004		Sample		ethanol quant.M
	49	30012020-A	0.400	Control		ethanol quant.M
ľ	50	14082019-B	0.040	Control	$a \sim 0$.	ethanol quant.M
Γ	51	4110320133/10	0.199	Control	-N-0. 2	ethanol quant.M
ſ	52	011823WB	Negative	Control	O' ZiO'	ethanol quant.M

Dissemination is restricted to rized horized horized horized horized authorized prosecutor agencies on a gencies to unauthorized agencies to unauthorized agencies to unauthorized agencies of scottsdale city prosecutor scottsdale city pro Dissemination is restricted to

Scottsdale Police Department Crime Laboratory Summary of Cases

SEQUENCE NAME: 22Feb23 ANALYST: Brooke

PB

Vials	Test 1 (g/dL)	Test 2 (g/dL)	Mean (g/dL)	Percent Difference*	Absolute Difference (g/dL)*
10 11	0.0000	0.0000	0.00000	0.00 7.	0.00000
12 13	0.0624	0.0621	0.06225	0.24	0.00015
14 15	0.2301	0.2331	0.23160	0.65	0.00150
16 17	0.1710	0.1731	0.17205	0.61	0.00105
18 19	0.0000	0.0000	0.00000	0.00	0.00000
21 22	0.2400	0.2402	0.24010	0.04	0.00010
23 24	0.0880	0.0871	0.08755	0.51	0.00045
25 26	0.1619	0.1605	0.16120	0.43	0.00070
27 28	0.2135	0.2141	0.21380	0.14	0.00030
29 30	0.2685	0.2643	0.26640	0.79	0.00210
32 33	0.1979	0,1983	0.19810	0.10	0.00020
34 35	0.1642	0.1627	0.16345	0.46	0.00075
36 37	0.1012	0.1013	0.10125	0.05	0.00005
38 39	0.1962	C0.1943	0.19525	0.49	0.00095
40 41	0.2057	0.2036	0.20465	0.51	0.00105
43 44	0.3568	0.3591	0.35795	0.32	0.00115
45 46	0.0902	0.0902	0.09020	0.00	0.00000
47 48	0.2802	0.2777	0.27895	0.45	0.00125

^{*}Calculated differences are differences from the mean of the two results.

8

ANALYST: Brooke SEQUENCE: 22Feb23

Instrument Position	Headspace Vial 1	Headspace Vial 2	Blood	Barcode Match
Vials 10 and 11	327-01A.B.	327-01A.B.	327-01A.B.	Yes
Vials 12 and 13	402-2R.E.	402-2R.E.	402-2R.E.	Yes
Vials 14 and 15	420-01A.G.	420-01A.G.	420-01A.G.	Yes
Vials 16 and 17	41902I.C.	7 41902I.C.	41902i.C.	Yes
Vials 18 and 19	423-01D.G.	423-01D.G.	423-01D.G.	Yes
Vials 21 and 22	422-01A.W.	422-01A.W.	422-01A.W.	Yes
Vials 23 and 24	387-01E.C.	387-01E.C.	387-01E.C.	Yes
Vials 25 and 26	423-01V.W.	423-01V.W.	423-01V.W.	Yes
Vials 27 and 28	2303054-2	2303054-2	2303054-2	Yes
Vials 29 and 30	2303044-16	2303044-1	2303044-1	Yes
Vials 32 and 33	2302949-1	2302949-1	2302949-1	Yes
Vials 34 and 35	2303151-4	2303151-4	2303151-4	Yes
Vials 36 and 37	2303161-2	2303161-2	2303161-2	Yes
Vials 38 and 39	2303142-2	2303142-2	2303142-2	Yes
Vials 40 and 41	VIAL00002	VIAL00002	VIAL00002	Yes
Vials 43 and 44	VIAL00001	VIAL00001	VIAL00001	Yes
Vials 45 and 46	VIAL00003	VIAL00003	VIAL00003	Yes
Vials 47 and 48	VIAL00004	VIAL00004	VIAL00004	Yes

User: pbrooke 2/24/2023



Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.016	168.966

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.436	183.929

User: pbrooke 2/24/2023

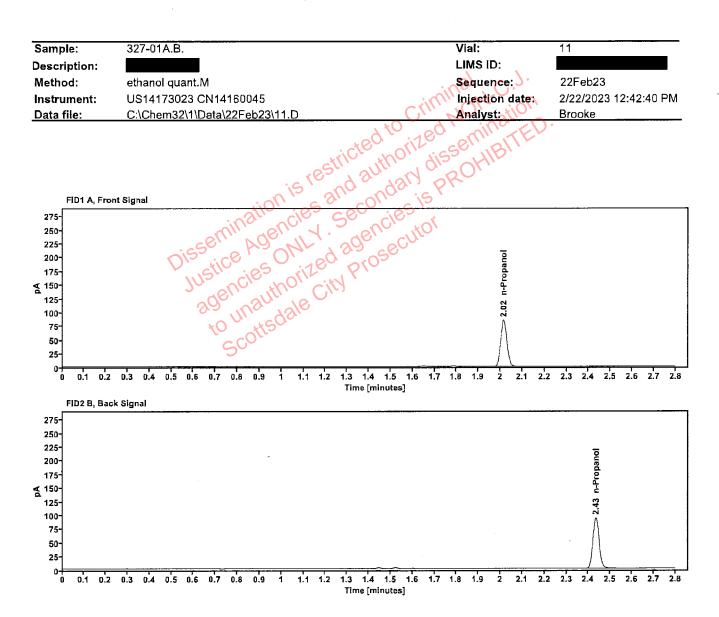


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.015	169.107


Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.435	184.015

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

402-1 R.E.

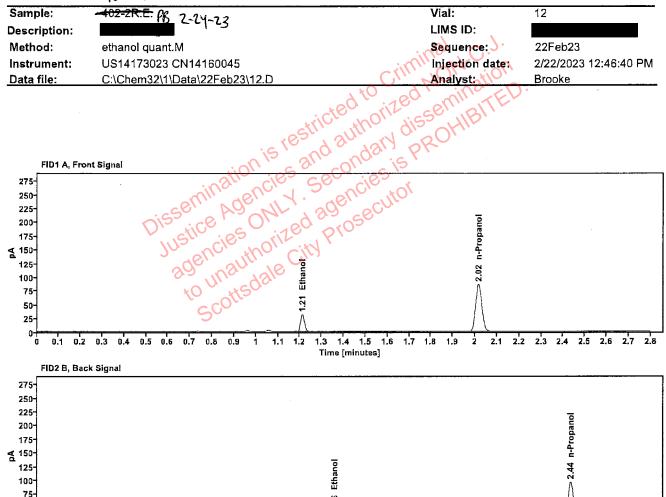

1.1 1.2

1.3 1.4 1.5 1.6 1.7 1.8 1.9

Time [minutes]

Table 1: FID 1 A (column DB-ALC1)

50-25-

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0624	1.212	39.676
n-Propanol		2.016	171.679

0.1 0.2 0.3 0.4 0.5 0.6 0.7 0.8 0.9

Table 2: FID 2 B (column DB-ALC2)

2.1 2.2

2.3 2.4

2.7


2


Compound	Time (min)	Peak Area
Ethanol	1.359	43.837
n-Propanol	2.436	186.816

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

402-1 R.E.



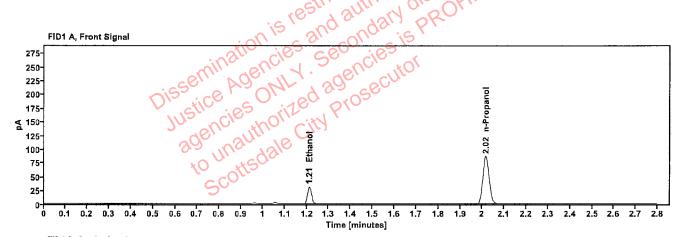

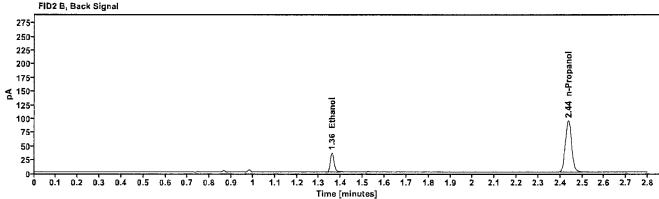


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0621	1.212	39.544
n-Propanol		2.016	171.915

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.360	43.664
n-Propanol	2.437	186.882

User: pbrooke 2/24/2023




Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2301	1.210	145.859
n-Propanol		2.016	169.952

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.357	161.288
n-Propanol	2.435	184.674

User: pbrooke 2/24/2023

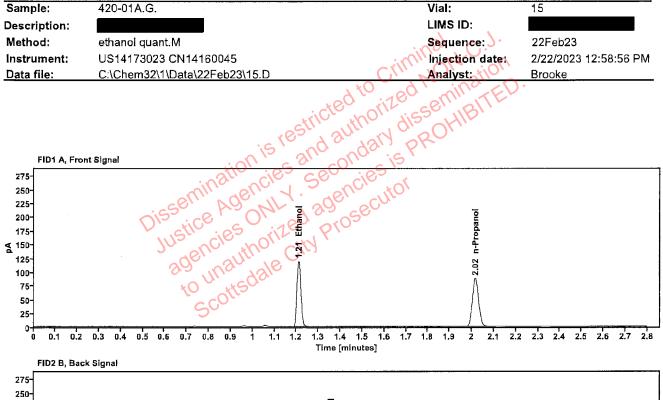

225-200-175-점 150-125-100-75-50-25-0.1 0.2 0.3 0.4 0.5 0.6 0.7 0.8 0.9 1.1 1.2 1.3 1.4 1.5 1.6 1.7 1.8 1.9 ż 2.1 2.2 2.3 2.4 2.5 2.6 2.7 2.8 Time [minutes]

Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2331	1.211	152.148
n-Propanol		2.017	174.991

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	168.154
n-Propanol	2.437	190.149

User: pbrooke 2/24/2023

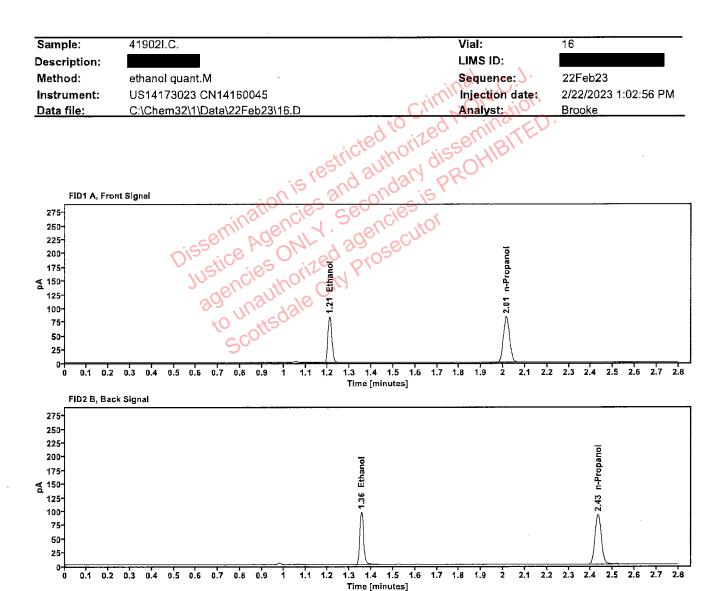


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1710	1.209	106.423
n-Propanol		2.014	166.992

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.355	116.281
n-Propanol	2.433	181.723

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

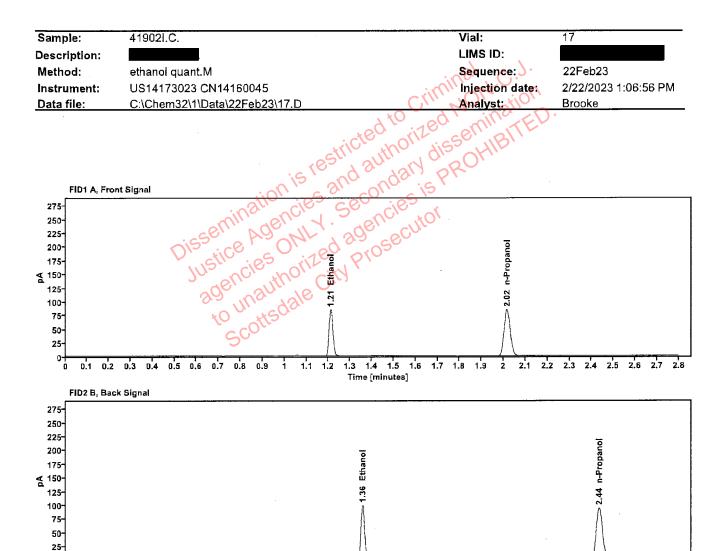

1.1 1.2

1.3 1.4 1.5 1.6 1.7 1.8 1.9

Time [minutes]

Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1731	1.210	108.297
n-Propanol		2.016	167.864

0.1 0.2 0.3 0.4 0.5 0.6 0.7 0.8 0.9

Table 2: FID 2 B (column DB-ALC2)

2.2

2.3 2.4

Compound	Time (min)	Peak Area
Ethanol	1.358	118.245
n-Propanol	2.436	182.646

Case: User: pbrooke 2/24/2023

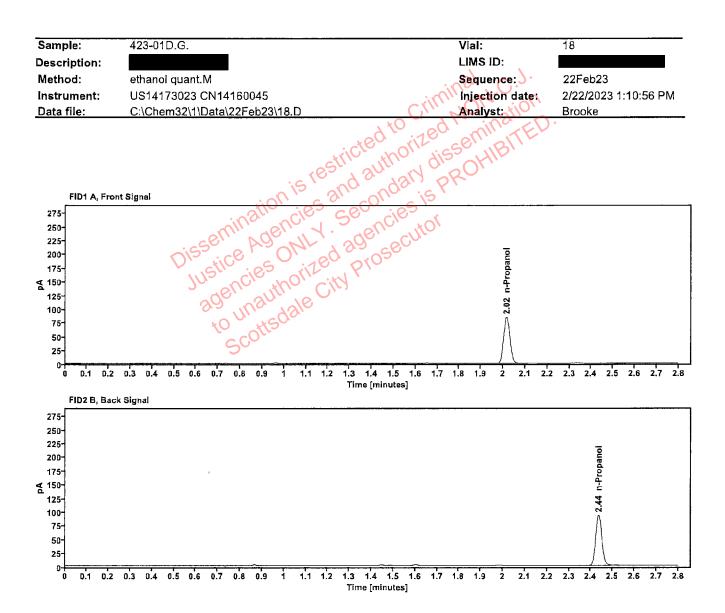


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.016	168.880

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.436	183,634

Case: User: pbrooke 2/24/2023



Table 1: FID 1 A (column DB-ALC1)

Compound	Amount	Time	Peak
	(g/100mL)	(min)	Area
n-Propanol		2.016	174.153

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
n-Propanol	2.437	189.897

User: pbrooke 2/24/2023

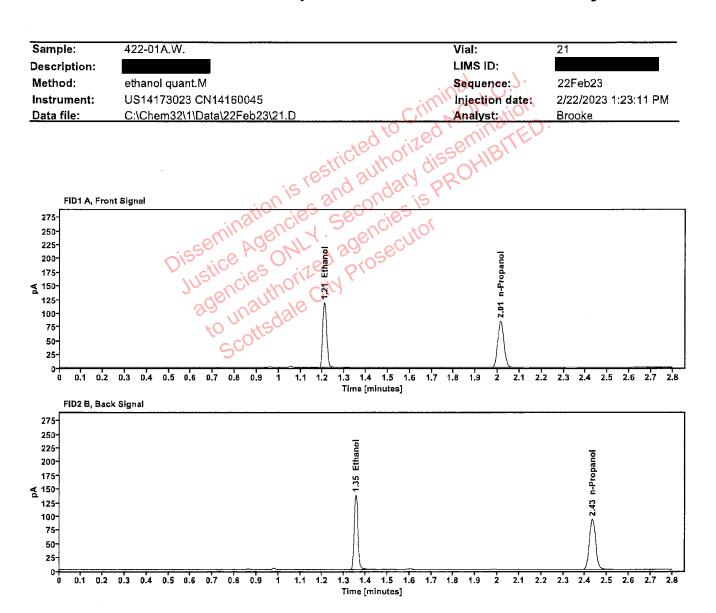


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2400	1.208	151.023
n-Propanol		2.014	168.683

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.354	165.582
n-Propanol	2.433	183.994

User: pbrooke 2/24/2023

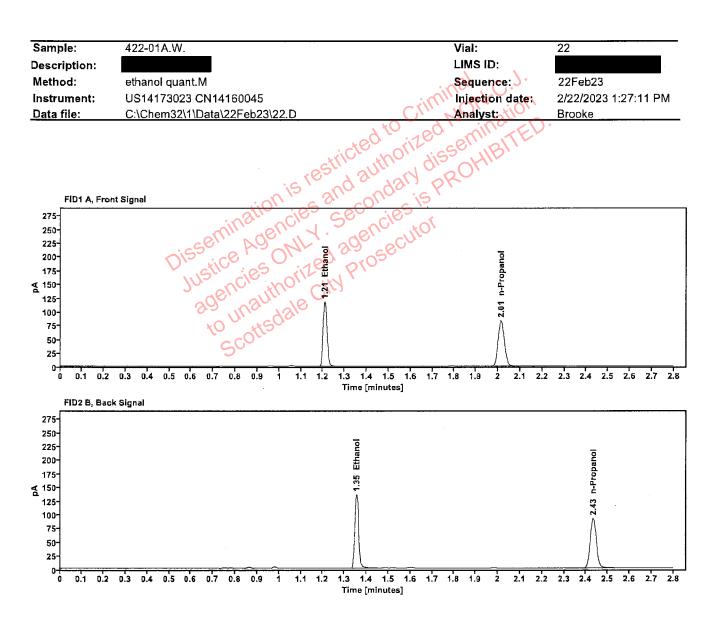


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2402	1.208	149.303
n-Propanol	w==	2.014	166.645

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.355	163.716
n-Propanol	2.433	181.502

User: pbrooke 2/24/2023

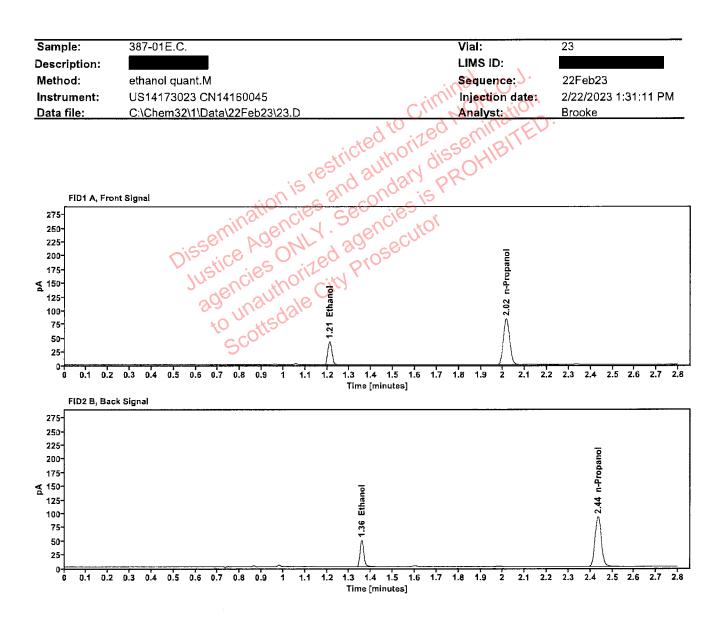


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0880	1.210	54.821
n-Propanol		2.015	167.813

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.357	59.934
n-Propanol	2.435	182.357

User: pbrooke 2/24/2023

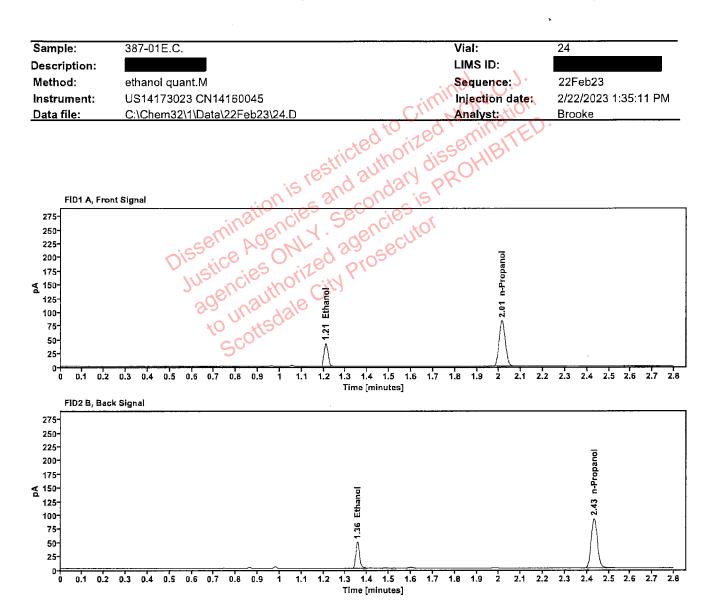



Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.D871	1.209	53.985
n-Propanol		2.014	166.950

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.356	59.107
n-Propanol	2.433	181.275

User: pbrooke 2/24/2023

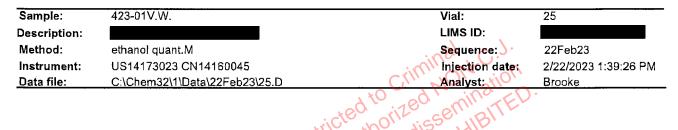

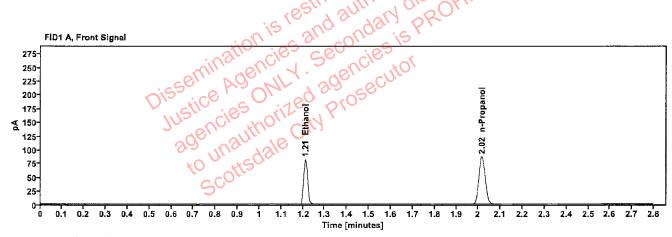

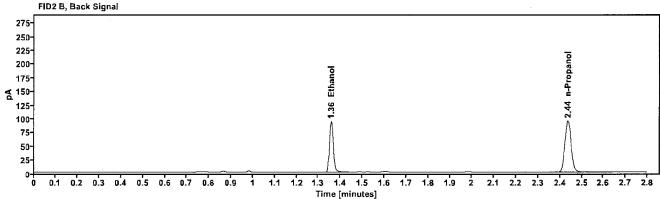


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1619	1.211	104.091
n-Propanol		2.016	172.547

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.358	113.713
n-Propanol	2.436	187.684

User: pbrooke 2/24/2023

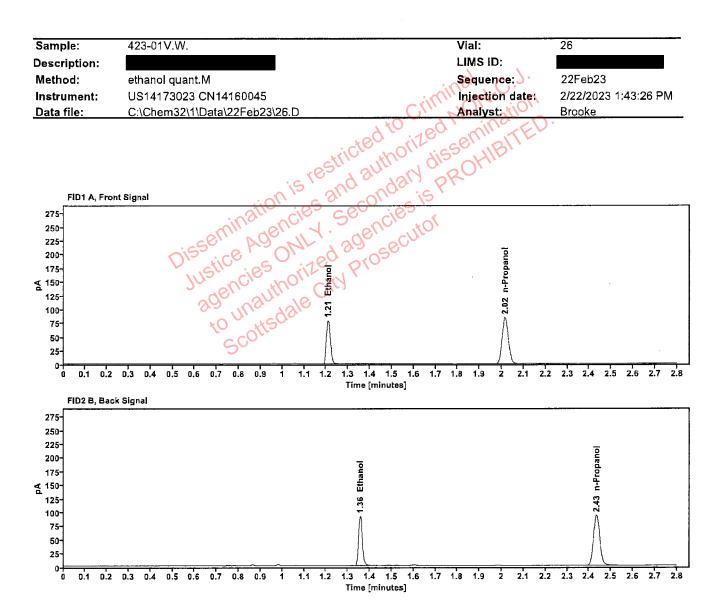


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1605	1.209	100.887
n-Propanol		2.015	168.714

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.356	110.458
n-Propanol	2.434	183.398

User: pbrooke 2/24/2023



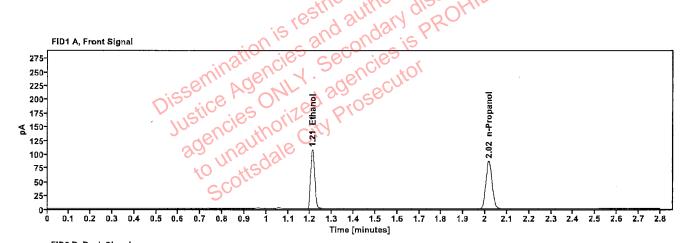

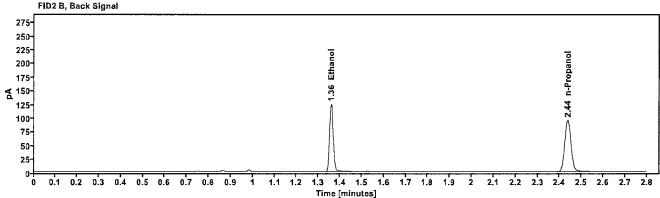



Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2135	1.211	137.630
n-Propanol		2.017	172.841

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	150.918
n-Propanol	2.437	187.362

User: pbrooke 2/24/2023



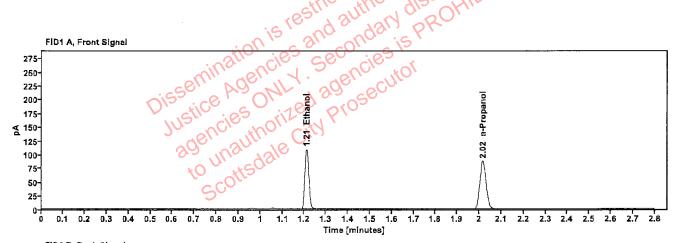

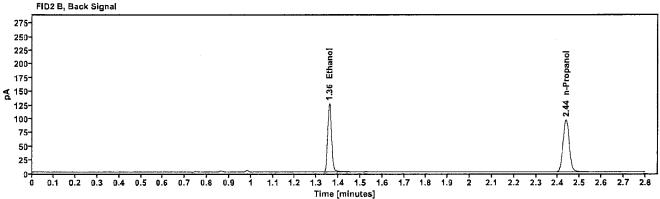


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2141	1.211	139.501
n-Propanol		2.017	174.707

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	152.502
n-Propanol	2.437	189.353

User: pbrooke 2/24/2023

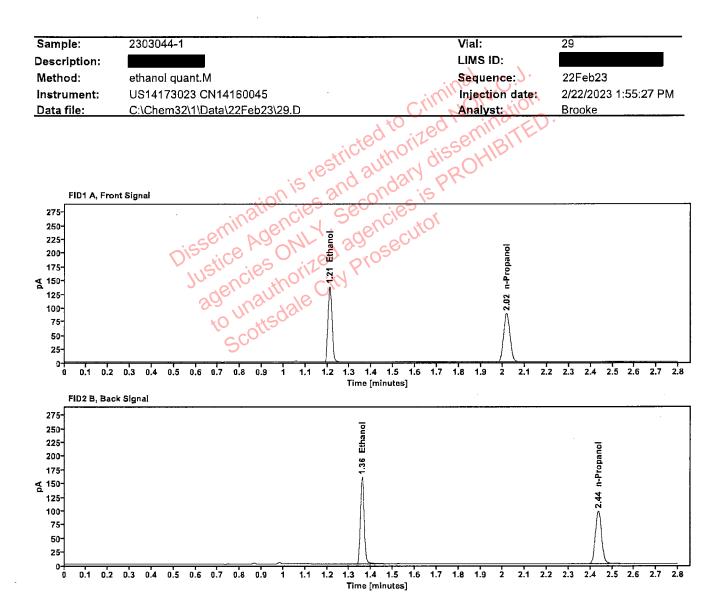


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2685	1.211	176.363
n-Propanol		2.016	176.039

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	193.426
n-Propanol	2.437	191.242

User: pbrooke 2/24/2023



Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2643	1.210	168.570
n-Propanol		2.016	170.928

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.358	185.106
n-Propanol	2.436	185.746

User: pbrooke 2/24/2023

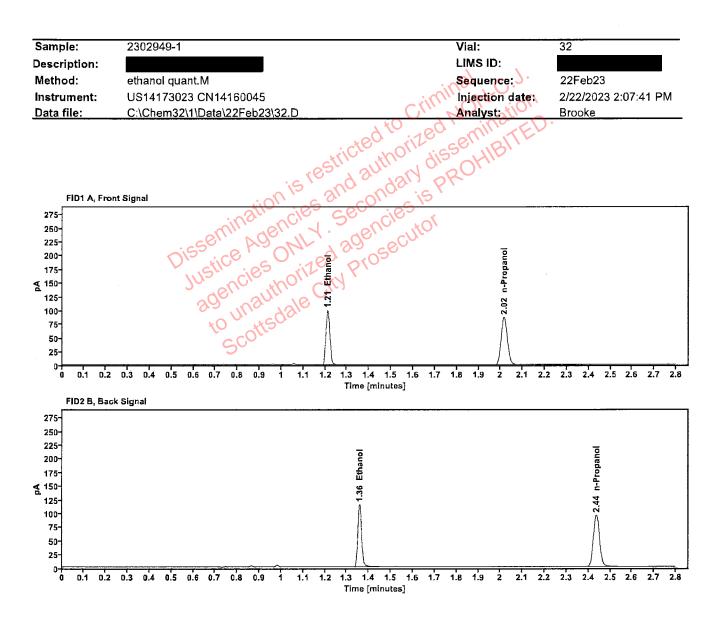



Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1979	1.211	127.314
n-Propanol		2.016	172.534

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	139.132
n-Propanol	2.437	187.359

User: pbrooke 2/24/2023

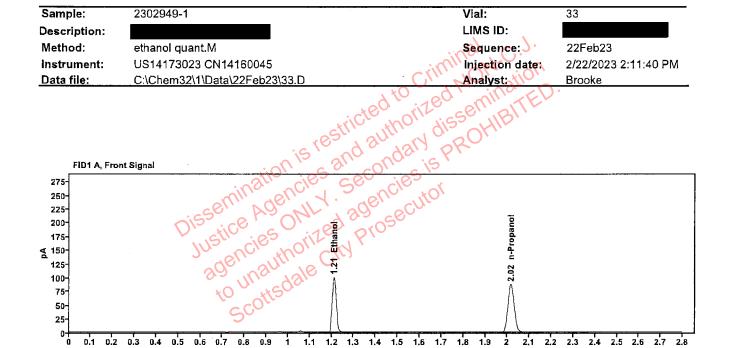

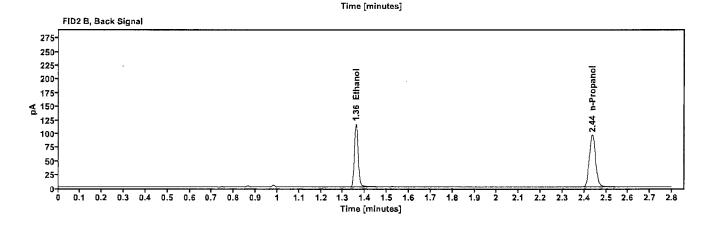


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1983	1.211	128.658
n-Propanol		2.017	174.005

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	140.741
n-Propanol	2.437	189.043

User: pbrooke 2/24/2023

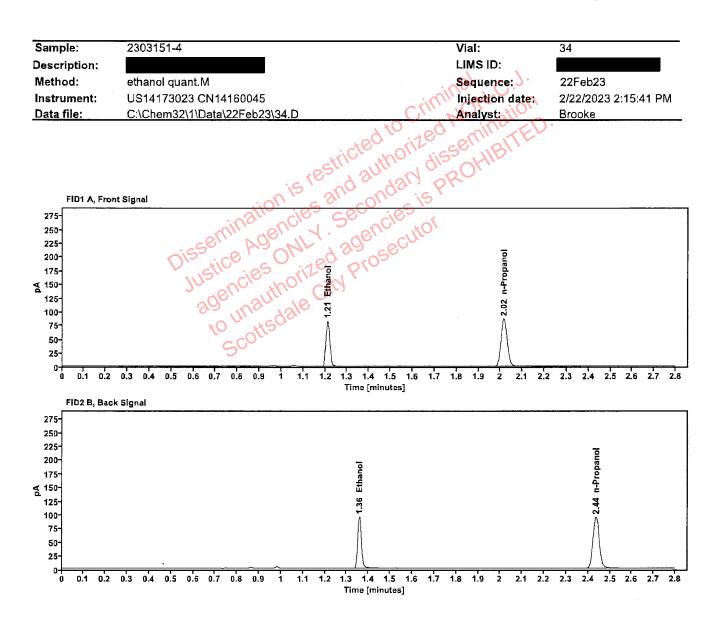


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1642	1.211	105.240
n-Propanol		2.016	172.050

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.358	114,966
n-Propanol	2.436	186.517

User: pbrooke 2/24/2023



Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1627	1.210	101.968
n-Propanol		2.015	168.240

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.357	111.389
n-Propanol	2,435	182.624

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

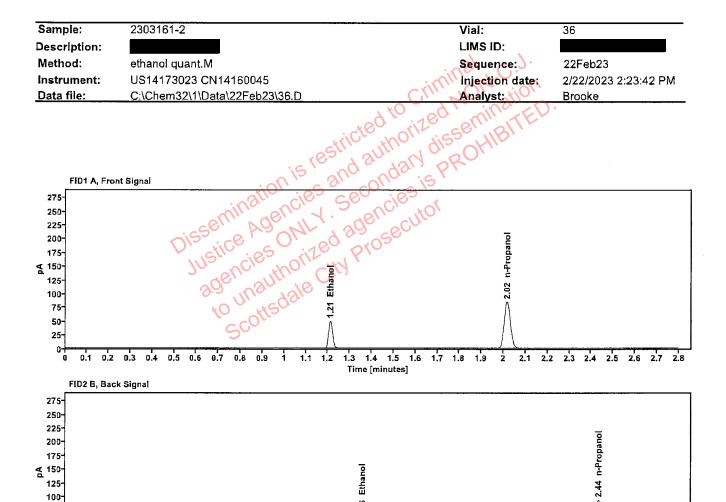

1.1 1.2 1.3 1.4 1.5 1.6 1.7 1.8 1.9

Time [minutes]

Table 1: FID 1 A (column DB-ALC1)

75-50-25-

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1012	1.211	63.452
n-Propanol		2.017	168.750

0.1 0.2 0.3 0.4 0.5 0.6 0.7 0.8 0.9 1

Table 2: FID 2 B (column DB-ALC2)

2.3 2.4

2 2.1 2.2

Compound	Time (min)	Peak Area
Ethanol	1.359	68.999
n-Propanol	2.437	183.084

User: pbrooke 2/24/2023

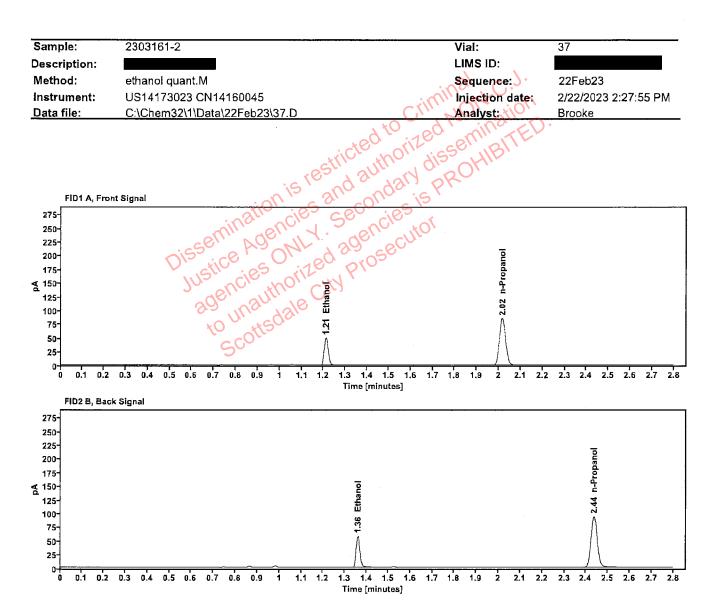


Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1013	1.212	64.185
n-Propanol		2.017	170.434

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.360	69.781
n-Propanol	2,437	184.775

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

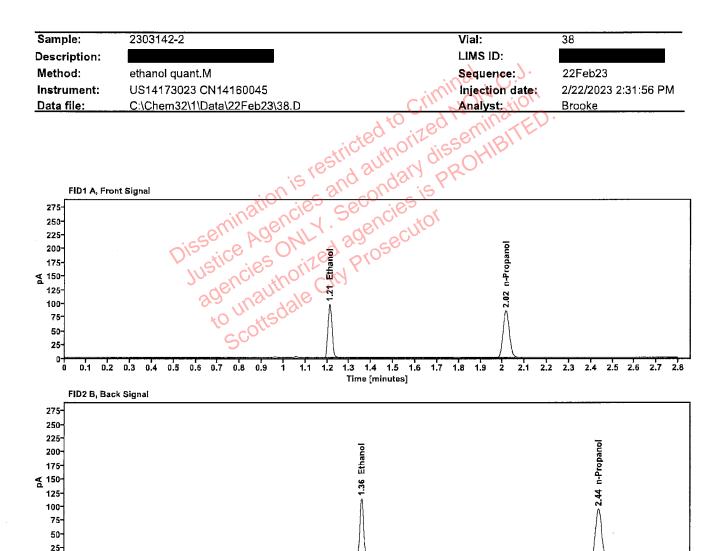

1.2 1.3 1.4 1.5 1.6 1.7 1.8 1.9

Time [minutes]

Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1962	1.211	124.937
n-Propanol		2.016	170.776

0.2 0.3 0.4 0.5 0.6 0.7 0.8 0.9

Table 2: FID 2 B (column DB-ALC2)

2.2

Compound	Time (min)	Peak Area
Ethanol	1.358	136.533
n-Propanol	2.436	184.966

User: pbrooke 2/24/2023



Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.1943	1.209	120.931
n-Propanol		2.015	166.925

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.356	131.977
n-Propanol	2.434	181.026

User: pbrooke 2/24/2023

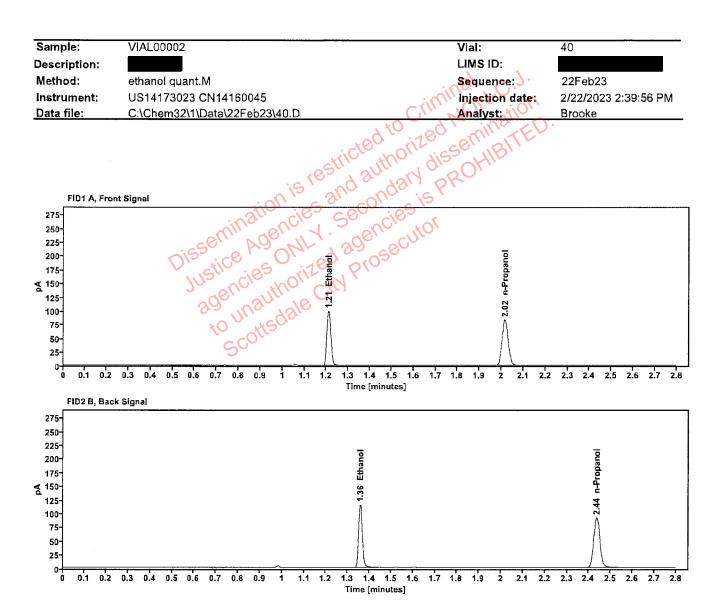


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2057	1.210	127.908
n-Propanol		2.016	166.763

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.358	139.863
n-Propanol	2.436	181.420

User: pbrooke 2/24/2023

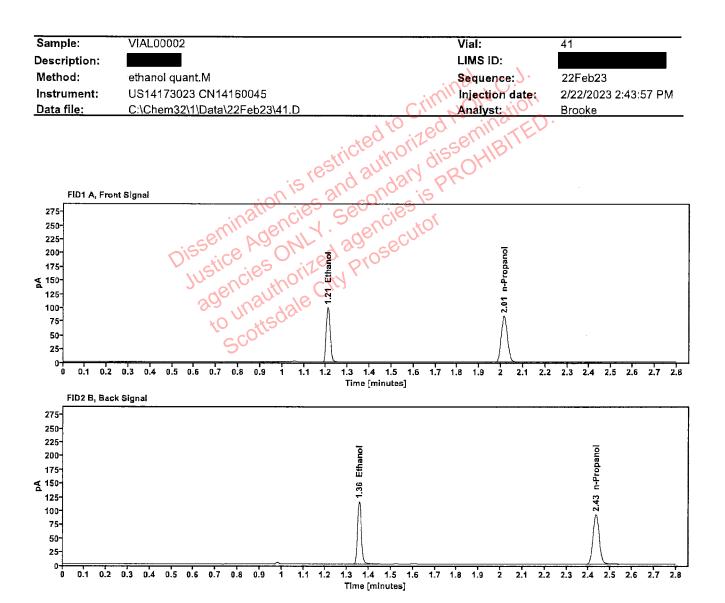


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2036	1.209	127.285
n-Propanol		2.015	167.638

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.356	139.388
n-Propanol	2.434	182.647

Case: User: pbrooke 2/24/2023

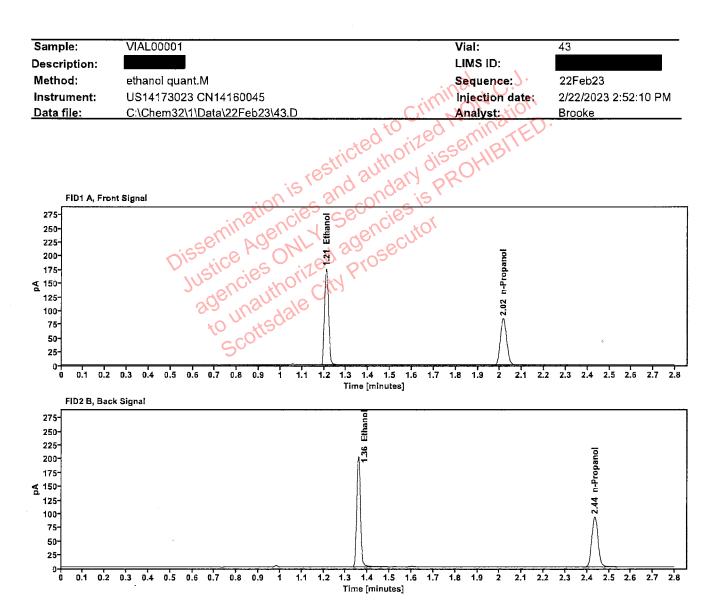


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.3568	1.210	224.186
n-Propanol		2.016	168.289

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.357	245.956
n-Propanol	2.436	183.304

Case: User: pbrooke 2/24/2023

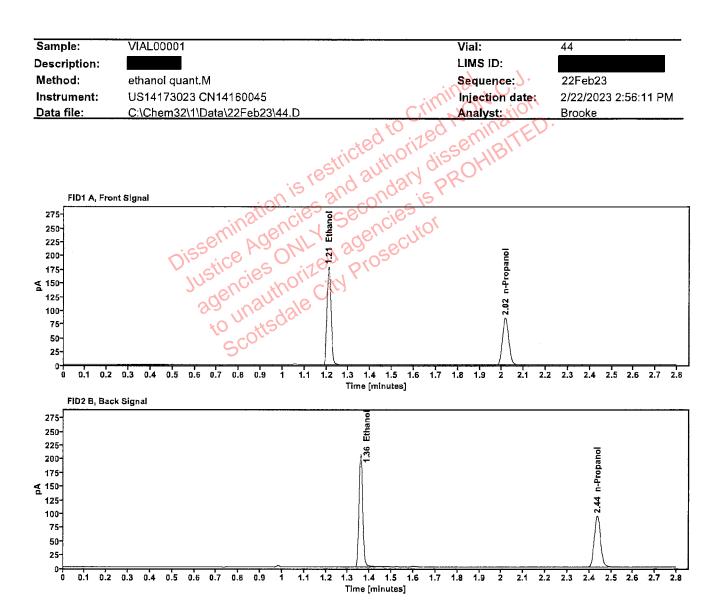


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.3591	1.210	228.498
n-Propanol		2.017	170.405


Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	250.865
n-Propanol	2.437	185.805

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

Sample: VIAL00003 Vial: 45 Description: LIMS ID: 22Feb23 Method: ethanol quant.M Sequence: Instrument: US14173023 CN14160045 Injection date: 2/22/2023 3:00:11 PM C:\Chem32\1\Data\22Feb23\45.D Data file: Brooke

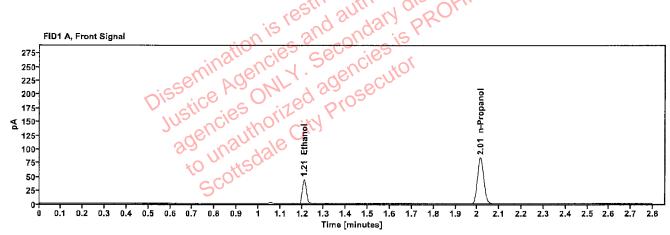

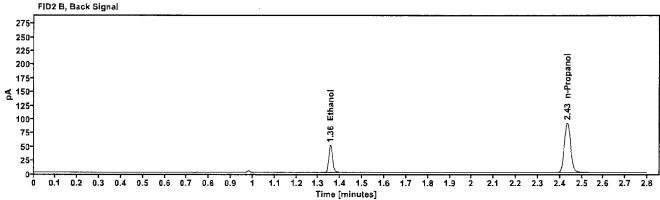



Table 1: FID 1 A (column DB-ALC1)


Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0902	1.210	55.783
n-Propanol		2.015	166.551

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.356	60.681
n-Propanol	2.434	181.466

User: pbrooke 2/24/2023



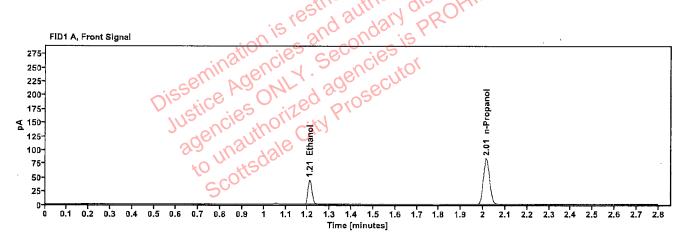

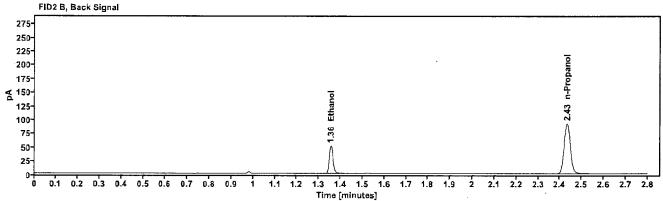


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.0902	1.209	56.206
n-Propanol		2.014	167.694


Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.356	61.063
n-Propanol	2.434	182.670

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

Sample: VIAL00004 Vial: 47 Description: LIMS ID: Method: ethanol quant.M Sequence: 22Feb23 Instrument: US14173023 CN14160045 Injection date: 2/22/2023 3:08:12 PM Data file: C:\Chem32\1\Data\22Feb23\47.D **Brooke**

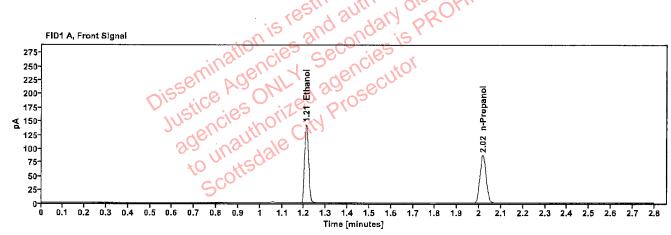

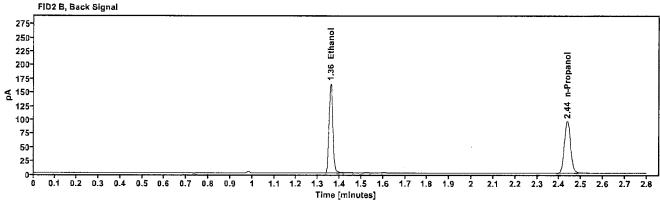


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2802	1.211	182.340
n-Propanol		2.017	174.381


Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.359	200.112
n-Propanol	2.437	189.882

User: pbrooke 2/24/2023

Scottsdale Police Department Crime Lab Volatiles Analysis

Sample: VIAL00004 Vial: 48 Description: LIMS ID: Method: ethanol quant.M Sequence: 22Feb23 Instrument: US14173023 CN14160045 Injection date: 2/22/2023 3:12:12 PM Data file: C:\Chem32\1\Data\22Feb23\48.D Analyst: Brooke

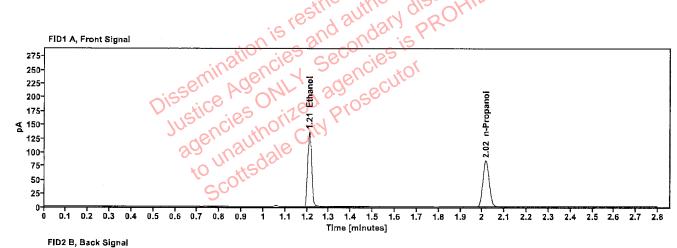

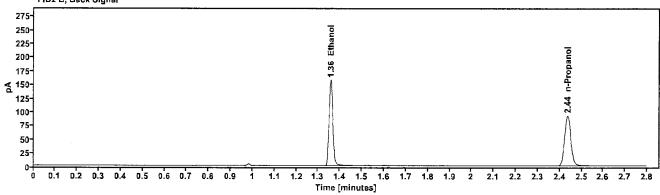


Table 1: FID 1 A (column DB-ALC1)

Compound	Amount (g/100mL)	Time (min)	Peak Area
>Ethanol	0.2777	1.210	173.773
n-Propanol		2.016	167.657

Table 2: FID 2 B (column DB-ALC2)

Compound	Time (min)	Peak Area
Ethanol	1.358	190.781
n-Propanol	2.436	182.491